

Instruments for Electrical Safety Compliance Testing



Experts In Electrical Safety Compliance.®

Hipot • Ground Bond • Insulation Resistance • Leakage Current • Functional Run Medical Test Systems • HV/HC Multiplexers • Software Solutions

CUSTOMER HAPPINESS PROMISE


We aim to provide an amazing experience and quality testers that last a long time. If you're not satisfied with your tester, return it within 45 days for a full refund. Calibrate annually with us, or one of our authorized partners, and we'll extend your warranty an additional year for the service life of your tester, and at least five years after discontinuation. If it breaks during that time, we promise to fix it for free (unless abuse or excessive damage is present). When your tester reaches the end of its service life, we'll responsibly recycle it and give you a discount on a replacement.



*Annual calibration and inspection must be made in each successive year starting one year after the original purchase date in order to remain eligible for extended warranty coverage beyond the standard warranty period (five years). (Not applicable for APCA region).

5 YEAR WARRANTY

Your new tester is warranted to be free from defects in workmanship and material for a period of (5) years from date of shipment.





ONGOING SUPPORT

We work to provide the best service and support in the industry. With decades of industry experience we are the pros you can trust to help you be compliant to NRTL standards. We'll work closely with you to help you achieve your goals. We've built a worldwide network of knowledgable partners, so you're covered no matter where you are.



A HISTORY OF INNOVATION

1936	Associated Research was founded.	2001	We released our patented safety feature, SmartGFI®, to provide our customers with
1939	We introduced the first battery operated Megohmmeter, the Vibrotest, in the United States.	2012	maximum operator protection during high voltage testing. We launched the first electrical
1966	We commenced the first Cable Testing/Fault Location school known as ARU. ARU continued for over 25 years.	2012	safety compliance analyzer with a built-in AC power source.
1993	We introduced the first complete family of microprocessor-controlled electrical safety	2013	We developed the first mobile app in the electrical safety testing industry.
1995	instruments. We developed the first multi-function electrical	2017	We launched the Applications Consulting program.
1997	we released the first electrical safety instrument with a built-in multiplexer for multi-point testing.	2020	We Introduced Withstand®, a Software as a Service (SaaS) platform, that is a cloud storage of your tests and data in one platform.
1999	We introduced Autoware, the first software package for automated instrument control,	2021	Associated Research joins the IKONIX family to become and IKONIX Brand.
	in the EST industry.	2023	Ikonix globalizes it's product portfolio.

FOCUSED ON EDUCATION

With over 80 years of industry experience, we have the resources and expertise to assist you with your educational needs throughout the life of your product.

- Quick Start Videos
 - On-Site Training
- Quick Start Guides White Papers & Articles

SERVING THE COMMUNITY



We donate a portion of our profits to raising awareness about the dangers of electricity.

PRODUCT REFERENCE CHART

















Hypot®			
3805	•		
3855	•		

		•

•	
•	•

Functional Run


Built-in AC Power

Hypot®				
3805	•			
3855	•			
3865	•	•		
3870	•	•		
HypotULTRA®				
7800	500 VA	•		
7804	•	•	•	
7820	•			
7850	•	•		
7854	500 VA	•	•	
OMNIA® II				
8204	•	•	•	
8254	500 VA	•	•	
8206	•	•	•	
8256	500 VA	•	•	
8207	•	•	•	
8257	500 VA	•	•	
HYAMP®				
3240			•	
HypotMAX [®]				
7705	•			
7710		•		
7715	•			
7720		•		
LINECHEK® II				
620L				
SC6540				
1181				

-	-				
•					
•	•				
•	•				
•	•				
•					
•	•				
•	•				
•	•				
•	•				
•	•	•	•		
•	•	•	•		
•	•	•	•	•	
•	•	•	•	•	

•			•

1111
НН
HG
GN
GG

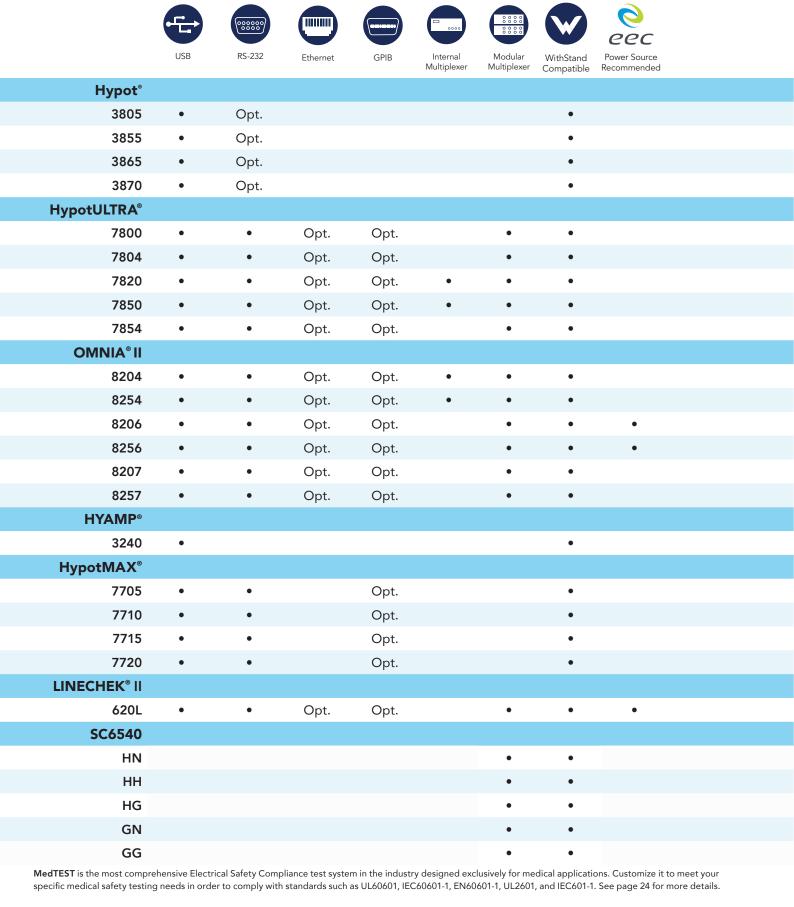



Our Hypot® Series raises the bar for production line Hipot testing. Improve traceability with onboard data storage and easily transfer test result data and test settings via convenient front panel USB. Take the guesswork out of your production line with the direct barcode connection to quickly associate products with pre-programmed test files. We've included advanced features like improved security and a touch screen interface that provides custom pop-up prompts displayed before each test step. We've dramatically reduced the weight and footprint of the Hypot® Series to make safety compliance a less strenuous ordeal. Quickly interconnect with the HYAMP® Series to form a complete safety compliance system.



Find the Model that Fits Your Testing Needs



SAFETY & PRODUCTIVITY **FEATURES**







SmartGFI[®] Automatic operator shock protection

Remote Safety Easily disable HV output

Easily import/ export test files and data via USB



Direct barcode

connection





Multiple Languages Multi-Language user interface



PLC Remote Basic PLC relay control



Prompt & Hold Provides alerts & instructions between tests



Advanced Customize ID & password protection



Interconnection Interconnect with HYAMP® to form a complete test system







Charge-LO® Confirms proper DUT



FailCHEK™ Confirms failure



Cal Accredited calibration

available



WithStand® Automation



On Board Data Storage Save up to 1,500 Test Results onhoard

INPUT SPECIFICATIONS		INSULATION RESISTANCE TEST MODE				
Voltage	100 – 120 VAC / 20	00 – 240 VAC ± 10% Au	to Range	Voltage Setting	Range:	30 – 1,000 VDC
Frequency	50/60 Hz ± 5%				Resolution: Accuracy:	1 V ± (1.5% of setting + 5 V)
Fuse	3.15 A, Fast Blow 2	250 VAC		Resistance Display	Range:	1 – 50,000 ΜΩ
DIELECTRIC WIT	HSTAND TEST M	1ODE			Resolution: 30 – 99 V	DC 100 – 499 VDC 500 – 1000 VDC
Output Rating	3805/3855/ 3865/3870	5 kVA @ 20 mAAC 6 kVA @ 7.5 mADC (3	865/3870 only)		MΩ MΩ 0.001 1.000 – 1. 0.01 2.00 – 19. 0.1 20.0 – 199. 1 200 – 10,0	MΩ MΩ MΩ .999 1.000 – 1.999 1.000 – 9.999 .99 2.00 – 19.99 10.00 – 99.99 .99 20.0 – 199.9 100.0 – 999.9
Maximum Limit	3805/3855/ 3865/3870	AC Range: Resolution:	0.00 – 20.00 mA 0.01 mA		Accuracy:	± (8% of reading+2 counts) at test voltage
		DC Range: Resolution: Accuracy:	0 - 7500 μA 1 μA AC and DC ± (2% of setting + 2 counts)		± (5% of readir	ng + 2 counts) for 1.00 – 999.9 M Ω ng + 2 counts) for 1000 – 9999 M Ω
Minimum Limit	3805/3855/ 3865/3870	AC Range: Resolution:	0.000 – 9.999 mA 0.001 mA	HI & LO-Limit	± (15% of read Range:	ing + 2 counts) for 10000 – 50,000 MΩ 0, 1.00 – 99.99 MΩ (0=OFF, HI-Limit ONLY)
		DC Range: Resolution: Accuracy:	0.0 – 999.9 μA 0.1μA AC and DC ± (2% of		Resolution:	0.01 MΩ 1000-50000 1 MΩ
			setting + 2 counts)		Range: Resolution:	100.0 – 999.9 MΩ 0.1 MΩ
Arc Detection	Range:	1 – 9 (9 is most sensit			Accuracy:	At test voltage 500-1000 V ± (2% of setting + 2 counts) for 1.00 – 999.9
Ground Fault Interrupt	·	150 μA max (AC or DC),	Fixed			MΩ \pm (5% of setting + 2 counts) for 1000 – 9999
	HV Shut Down Spe					$M\Omega$ ± (15% of setting + 2 counts) for 10000 –
Current Display	3805/3855/ 3865/3870	AC Range 1: Range 2:	0.000 – 4.000 mA 3.50 – 20.00 mA	Charge-LO	Range:	50,000 MΩ 0.000 – 3.500 μA DC or Auto Set
		DC Range 1: Range 2: Range 3:	0.0 μA – 400.0 μA 0.350 mA – 4.000 mA 3.50 mA – 7.50 mA	Ramp Timer	Range:	Ramp-Up: 0.1 – 999.9 sec Ramp-Down: 0, 1.0 – 999.9 sec, (0=OFF)
		Accuracy:	All Ranges ± (2% of read-	Delay Timer	Range:	0.5 – 999.9 sec (0=OFF)
DC Output Binale	4 F0/ Dia ala assa sa	L / LVDC @ 7.5 A D	ing + 2 counts)	Dwell Timer	Range:	0, 0.5 – 999.9 sec (0=continuous)
DC Output Ripple		t 6 kVDC @ 7.5 mA Resi	stive Load	GENERAL SPECIFICA	ATIONS	
RAMP-HI Selectable	Range: 0.0 – 7,500	μA, User Selectable		Remote Control and Signal I/O	Inputs: Test, Reset, Hardware Interlock, File Recall Outputs: Pass, Fail, Test-in-Process, Reset-Out, Start-Out	
Charge-LO	0 – 350 μA DC or A			Vmax	Displays the maximum voltage value recorded during a breakdown	
Discharge Time		oad, < 100 msec for ca pacitive load vs. outpu 0.08µF < 4KV		Imax	Displays the maximum leakage current value read during a test	
	0.75μF < 2KV 0.5μF < 3KV	0.04µF < 5KV 0.015uF < 6KV		Memories	50 steps 1500 test results	
AC Voltage Waveform/	Sine Wave, Crest F	Factor = 1.3 – 1.5		Interface	USB standard	
Frequency	Range:	50 or 60 Hz, User Sele		Language		al Chinese, Simplified Chinese, Turkish, ish, German, French
Dwell Timer	Range:	AC 0, 0.2-999.9 sec (0 DC 0, 0.4-999.9 sec (0		Security		ps with ID and password
Ramp Timer	Range:	Ramp-Up: 0.1 – 999.9 Ramp-Down: AC 0.0 - DC 0, 1.		Dimensions (W x H x D)	3805/3855/ 3865/3870	8.5" x 3.5" x 11.9" (215 mm x 88.1 mm x 300 mm)
Ground Continui- ty Current	DC 0.1A ± 0.01 A,	fixed		Weight	3805/3855/ 3865/3870	12 lbs (5.46 kgs)
Ground Conti- nuity Maximum Limit Minimum Limit	Range: Resolution: Accuracy:	$0.00 - 1.50 \Omega$ 0.01Ω ± (3% of setting + 0.0	12 Ω)	provide a better indication	of the instrument's st resolution of the o	ations using "counts" which allows us to see capabilities across measurement ranges. display for a given measurement range. For n 2 counts = 2 V.
Ground Conti- nuity Auto Offset	Range: Resolution: Accuracy:	$0.00 - 0.50 \Omega$ 0.01Ω ± (3% of setting + 0.0	2 Ω)	Specifications subject to	_	

HypotULTRA®


The Most Flexible and Feature-Rich Automated Dielectric Analyzer Available



Our HypotULTRA® models provide all the tools you need to modernize your production line with best-in-class 4-in-1 test capability and a slim 2U design. We've added 40A AC Ground Bond test capability to HypotULTRA's already impressive feature list for manufacturers that aim to adopt best testing practices without sacrificing productivity. Whether you're looking to improve traceability with onboard data storage, increase efficiency with our intuitive touch screen interface and direct barcode scanner connection, or automate with a variety of communication interfaces, HypotULTRA was designed to take your production line to the next level.



Find the Model that Fits Your Testing Needs

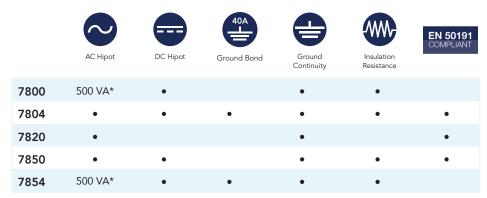

^{*}Meets 200 mA short circuit requirements

AVAILABLE INTERFACES









Ethernet RS-232

SAFETY & PRODUCTIVITY







SmartGFI[®] Automatic

operator shock protection

Easily disable HV output

Easily import/ export test files and data via USB



Capability Direct barcode connection



Multiple Languages Multi-Language use interface



Ground Bond Voltage Drop voltage drop



ProVOLT® Multi-dwell cycles at different ACW/DCW/IR



Multiplexer Available with optional HV (4 or 8 ports)



Multiplexer Compatible with SC6540





failure

detection



Prompt & Hold Provides alerts & instructions

between tests



WithStand® Automation Software



User Security

Customize ID & password

protection





Reduce ramp DC Hipot connection





Basic PLC relay control



Negative DC Hipot Reverse polarity DC Hipot (optional)



On Board Data Storage Save up to 100,000 Test Results onboard

HypotULTRA® Series

MOUNT 10 10 10 10 10 10 10 1							HypotULTRA® Series
Property Property	INPUT SPECIFICA	ATIONS			INSULATION RESISTA	NCE MODE	(Models 7800/7804/7850 & 7854 Only)
Property 1906 14 17 17 17 17 17 17 17	Voltage	100 – 120 VAC /	200 – 240 VA	AC ± 10% Auto Range	5 5	0 mA peak	
Page	Frequency	50/60 Hz ± 5%			and LO-Limit		
Control Cont	Fuse	7804					
Part	AC WITHSTAND	TEST MODE (#		15A, Fast Blow 250 VAC		Resolution:	0.1 ΜΩ
Deptit Program Deptit Program Deptit Program Support Deptit Program Support Program Support Deptit Program Support Deptit Program Support Program Support Deptit Program Support Program Sup	Output Voltage	Resolution:	1 VAC			Range:	1,000 ΜΩ – 50,000 ΜΩ
Mapped	Output Frequency	-		-			
Manual Cultum Table Range 10 - 19979 sec 10 - 19					Ramp Up Timer	Range:	0.1 – 999.9 sec
	· ·				Ramp Down Timer	Range:	1.0 – 999.9 sec
Charge-LO Cha	lation	= (170 of output	1 3 7 7		Dwell Timer	Range:	0.5 – 999.9 sec (0=Continuous)
Part		Total		0.001 mA	Delay Timer	Range:	0.5 – 999.9 sec
Part				Models 7800/7854)	Charge-LO	0.000 – 3.500	μA or Auto Set
Part				± (2% of setting + 2 counts)	CONTINUITY TEST M	ODE (All Mod	dels)
Residuation Dot Dot Property Dot Property Dot Dot Property Dot Dot Property Dot			racy:	± (2% of setting + 6 counts) 7800/7854	Output Current, DC	0.01 A for 10.0	01 – 100 Ω, 0.001 A for 101 – 1,000 Ω
Ramp Up Timer Ramp Country Ram		Real	Resolu- tion: Range: Resolu-	0.001 mA 10.00 – 40.00 mA (10 – 99.99 mA 7800/7854) 0.01 mA	& Min	Resolution:	0.001 Ω
Devel Timer Range 0, 0.2 - 9999 yes c 0-Cardinuous Asc Percentage			Accuracy: 0.1 – 999.9 s	ec		Resolution:	0.01 Ω
Note	Dwell Timer	Range:	e: 0, 0.2 – 999.9 sec (0=Continuous)			Resolution:	0.1 Ω
Accuracy Range 1 - 9 (9 is most sensitive) Range 1.0% of setting + 3 counts) Range Range 1.0% of setting + 5 v)						Range:	
DC WITHSTAND TEST MODE Models 7800/7804/7850 & 7854 Only) Resolution: 1.2 Accuracy: 2.7% of setting + 10 counts) Counts (Ripple Macuracy: 2.7% of setting + 10 counts) Counts (Ripple Macuracy: 2.7% of setting + 10 counts) Counts (Ripple Macuracy: 2.7% of setting + 10 counts) Counts (Ripple Macuracy: 2.7% of setting + 10 counts) Counts (Ripple Macuracy: 2.7% of setting + 10 counts) Counts (Ripple Macuracy: 2.7% of setting + 10 counts) Counts (Ripple Macuracy: 2.7% of setting + 10 counts) Counts (Ripple Macuracy: 2.7% of setting + 10 counts) Counts (Ripple Macuracy: 2.7% of setting + 10 counts) Counts (Ripple Macuracy: 2.7% of setting + 10 counts) Counts (Ripple Macuracy: 2.7% of setting + 10 counts) Counts (Ripple Macuracy: 2.7% of setting + 2 counts) Counts (Ripple Macuracy:							
Output Voltage			Range: 1 – 9 (9 is most sensitive)				
DC Output Ripple				•			
DC Output Ripple C4% (6 KV/10 mA at Resistive Load) Resistance Offset Range: 0.000 − 1.000 Ω Resistance Offset Range: 0.000 − 1.000 Ω Resistance Offset Range: 0.000 − 1.000 Ω − 1.000 Ω − 1.000 − 1.0	Output Voltage	Resolution:	1 V		Dwell Timer	Range:	0, 0.4 – 999.9 sec (0=Continuous)
Range:	DC Output Ripple			-	Resistance Offset	Range:	0.000 – 10.00 Ω
Accuracy 2 % of setting + 10 counts), Low Range is ON Resolution: Accuracy 2 (2 % of setting + 3 counts) Open Circuit					GROUND BOND TEST	T MODE (Mo	dels 7804 & 7854 Only)
Resolution: Accuracy: ± (2% of setting + 10 counts), Low Range is ON Range: Resolution: 0.01 μA Accuracy: ± (2% of setting + 10 counts), Low Range is ON Accuracy: ± (2% of setting + 10 counts), Low Range is ON Maximum Loading 1.00 - 10.00 A, 0 - 200 mΩ 1.00 - 200 mΩ 1.		Accuracy:	± (2% of set	-		Resolution:	0.01 VAC
Resolution 0.01 μA Accuracy ± (2% of setting + 10 counts), Low Range is ON		Resolution: Accuracy:	0.001 µA ± (2% of set	ting + 10 counts), Low Range is ON	Output Current	Resolution:	0.01 A
Range Resolution: Accuracy: ± (2% of setting + 2 counts) HI and LO-Limit Range: 0 - 150 mΩ (pr 3.0.1 - 40.00 A 0 - 600 mΩ (pr 1.0.0 - 10.01 A 1 mΩ 1.0.0 - 10.000 μA range (7804/54) 1.0.00 - 10.000 μA range (7804/54) 1.0.00 - 10.000 μA range (7806/50) 2.0.00 μA r		Resolution:	0.01 µA ± (2% of set	ting + 10 counts), Low Range is ON	Maximum Loading	1.00 – 10.00 A	- , 0 – 600 mΩ
1000		Resolution:	0.1 uA	r	HI and LO-Limit	30.01 – 40.00	A, 0 – 150 mΩ
Ramp Down Timer Range: 0.0, 1.0 – 999.9 sec (0=OFF) Dwell Timer Range: 0.0, 1.0 – 999.9 sec (0=Continuous) 0, 1.0 – 999.9 sec (0=Continuous) 0, 1.0 – 999.9 sec (0=Continuous) Milliohm Offset 0 – 200 mΩ		Resolution:	1,000 – 10,0 1 µA	00μA range (7800/50)			$0-600~\text{m}\Omega$ for 1.00 – 10.01 A 1 m Ω
Dwell Timer Range: 0., 0.4 – 999.9 sec (0=Continuous) Dwell Timer Range: 0, 0.4 – 999.9 sec (0=Continuous) 0, 1.0 – 999.9 sec, Low Range is ON Milliohm Offset 0 – 200 mΩ Ramp-HI Selectable Range: 0 – 20 mA selectable Voltage Offset 0.0 - 6.0 V Charge-LO Range: 0.0 – 350.0 μA DC or Auto Set GENERAL SPECIFICATIONS Discharge Time < 50 ms for no load, < 100 ms for capacitive load Memory 2,000 steps, 200 steps per test file max 100,000 test results Maximum Capacitive Load DC Models 75 μF < 2 kV 0.04 μF < 5 kV 0.015 μF < 6 kV Mechanical Bench or rackmount (2U height) with feet Arc Detection Range: 1 – 9 (9 is most sensitive) Standard: USB, RS-232 Optional: GPIB (IEEE-488.2), Ethernet or USB Printer INSULATION RESISTANCE MODE (Models 7800/7804/7850 & 7854 Only) Meight Milliohm Offset Mechanical SmartGFIP O, 0.4 – 5.0 mA (0=OFF) Dimensions (W x H x D) 16.92" x 3.50" x 15.75" (430 x 88.1 x 400mm) 45 lbs (20.4 kg) 7800: 41 lbs (15.4 kg) 7850: 43 lbs (15.9 kg) Part of the print of the pr	Ramp Up Timer	Range:	0.5 – 999.9 s	sec, Low Range is ON		Resolution:	1 mΩ
Range: 0, 44 - 999,9 sec, Low Range is ON Milliohm Offset 0 - 200 mΩ					Dwell Timer	,	
Charge-LO Range: 0.0 - 350.0 μA DC or Auto Set	Dwell Timer	Range:	0, 0.4 – 999. 0, 1.0 – 999.	9 sec (U=Continuous) 9 sec, Low Range is ON			5, 2.2
$ \begin{array}{llllllllllllllllllllllllllllllllllll$		Range:	0 – 20 mA se	electable	Voltage Offset	0.0 - 6.0 V	
Maximum Capacitive Load DC Mode 1μF < 1kV 0.75 μF < 2 kV 0.04 μF < 5 kV 0.015 μF < 6 kV	Charge-LO	Range:	0.0 – 350.0 µ	JA DC or Auto Set	GENERAL SPECIFICA	TIONS	
Maximum Capacitive Load DC Mode $1 \mu F < 1kV \\ 0.75 \mu F < 2 kV \\ 0.5 \mu F < 3 kV \\ 0.015 \mu F < 6 kV$ $0.0 \mu F < 4 kV \\ 0.015 \mu F < 5 kV \\ 0.015 \mu F < 6 kV$ Mechanical Bench or rackmount (2U height) with feet Arc Detection Range: $1 - 9$ (9 is most sensitive) Interface Standard: USB, RS-232 Optional: GPIB (IEEE-488.2), Ethernet or USB Printer INSULATION RESISTANCE MODE (Models 7800/7804/7850 & 7854 Only) Output Voltage, DC Range: 10 - 1,000 VDC Accuracy: $1 - 1,000 \text{ VDC}$ (1.5% of setting + 2 counts) Dimensions (W x H x D) 16.92 " x 3.50" x 15.75" (430 x 88.1 x 400mm) Weight 7800: 7800: 7800: 7800: 7800: 7804: 7804: 7800: 7804: 7804: 7806: 7804: 7806: 7804: 7806: 7804: 7806: 7804: 7806:	Discharge Time	< 50 ms for no l	oad, < 100 m	s for capacitive load	Memory		
Name	Capacitive Load	$0.75 \mu F < 2 kV$	$0.04 \mu F < 5$	kV	Mechanical		
NSULATION RESISTANCE MODE (Models 7800/7804/7850 & 7854 Only) SmartGFI® 0, 0.4 – 5.0 mA (0=OFF)					Interface		
Output Voltage, DC Resolution: 1 VDC Accuracy: ± (1.5% of setting + 2 counts) Range: Range: 1,001 – 6,000 VDC Resolution: 1 VDC Resolution: 1 VDC Resolution: 1 VDC Resolution: 1 VDC Resolution: 1 VDC Resolution: 1 VDC Dimensions (W x H x D) 16.92" x 3.50" x 15.75" (430 x 88.1 x 400mm) Weight 7800: 45 lbs (20.4 kg) 41 lbs (18.6 kg) 7804: 41 lbs (18.6 kg) 7850: 34 lbs (15.4 kg) 7850: 35 lbs (15.9 kg) 7854: 44 lbs (21.4 kg)		-			SmartGFI®		
Resolution: 1 VDC				•			
Range: 1,001 – 6,000 VDC 7850: 35 lbs (15.9 kg) Resolution: 1 VDC 7854: 46.2 lbc (21 kg)	DC	Resolution:	1 VDC		· · · · · ·	7800: 7804:	45 lbs (20.4 kg) 41 lbs (18.6 kg)
		Resolution:	1 VDC			7850:	34 lbs (15.4 kg) 35 lbs (15.9 kg)


Specifications subject to change without notice.



Our OMNIA® II Series is a complete line of multi-function electrical safety compliance analyzers designed to satisfy even the most demanding application requirements. We've included exclusive productivityenhancing features and the latest in safety technology to make this product line the envy of the industry. With 6 models to choose from, a multi-language menu system and a variety of automation interfaces available, the OMNIA® II is ready for global deployment.



Find the Model that Fits Your Testing Needs

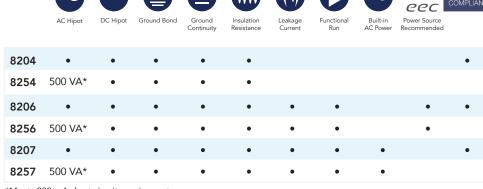

*Meets 200 mA short circuit requirements

AVAILABLE INTERFACES









GPIB

SAFETY & PRODUCTIVITY FEATURES







SmartGFI[®] Automatic

Easily disable HV output protection

Hold Provides alerts & instructions between tests



Language user interface





Active Link® Continuous power during test steps



Customize your own shortcut







Multiplexer Available with optional HV multiplexer (8 ports)



Multiplexer Compatible with SC6540 multiplexers







FailCHEK™ Confirms failure detection



Cal-Alert® Tracks and alerts for calibration



Reduce ramp

DC Hipot





Confirms High proper DUT frequency connection filter for corona



Automation



Accredited Accredited calibration available



detection

Ground Bond Voltage Drop Monitor vs resistance

INPUT SPECIFICA				
Voltage	115/230 V Aut	o Range, ± 15	% Variation	
Frequency	50/60 Hz ± 5%	50/60 Hz ± 5%		
Fuse	115 VAC, 230	VAC – 10 A Slo	ow Blow 250 VAC	
DIELECTRIC WIT	HSTAND TES	T MODE		
Output Rating	5 kV @ 50 mA 5 kV @ 100 mA 6 kV @ 20 mA	AAC (Models	825X)	
Voltage Setting	Resolution: Accuracy:	1 V ± (1.5% of se	etting + 5 volts)	
HI and LO-Limit	AC Total	Range: Resolution:	0.000 – 9.999 mA 0.001 mA	
		Range: Resolution:	10.00 – 50.00 mA (100.00 mA, models 825X) 0.01 mA	
		Accuracy:	± (2% of setting + 2 counts)	
	AC Real	Range: Resolution:	0.000 – 9.999 mA 0.001 mA	
		Range: Resolution:	10.00 – 50.00 mA (100.00 mA, models 825X) 0.01 mA	
		Accuracy:	± (3% of setting + 50 μA)	
	DC	Range: Resolution:	0 – 999.9 μA 0.1 μA	
		Range: Resolution:	1,000 – 20,000 μA 1 μA	
		Accuracy:	± (2% of setting + 2 counts)	
Arc Detection	Range:	1 – 9 (9 is m	ost sensitive)	
Ground Continuity	Current: DC 0 Max. Ground		fixed $\Omega \pm 0.1 \Omega$, fixed	
Ground Fault Interrupt	GFI Trip Curre HV Shut Down		i.0 mA (AC or DC)	
DC Output Ripple	≤ 4% Ripple rı	ms at 5 kVDC	at 20 mA Resistive Load	
Discharge Time	≤ 50 ms No Lo	oad, < 100 ms	for Capacitive Load	
Max Capacitive Load, DC Mode	1 μF < 1 kV 0.75 μF < 2 kV 0.5 μF < 3 kV		.08 μF < 4 kV .04 μF < 6 kV	
AC Output Waveform	Sine Wave, Cr	est Factor = 1	.3 – 1.5	
Output Fre- quency	Range:	60 or 50 Hz,	User Selection (400/800 Hz optional)	
Output Regu- lation	± (1% of outpo		no load to full load and over input	
Dwell Timer	Range: Range:		9 sec (0=Continuous) 9 sec (0=Continuous)	
Ramp Timer	Ramp-up: Ramp- Down:		.9 sec, DC 0.4 – 999.9 sec .9 sec, DC 0.0 , 1.0 – 999.9 sec pus)	
INSULATION RE	SISTANCE TE	ST MODE		
Voltage Setting	Range:	30 – 6000 VI	DC	
HI and LO-Limit	Range: Resolution:	0.05 MΩ – 9 0.01 MΩ	9.99 ΜΩ	
	Range: Resolution:	100.0 MΩ – 0 0.1 MΩ	999.9 ΜΩ	
	Range: Resolution:	1,000 MΩ – 1 1 MΩ (HI-Lin		
Ramp Timer	Ramp-up: Ramp- Down:	0.1 – 999.9 so 0.0, 1.0 – 999	ec 9.9 sec (0=Continuous)	

GROUND BOND	TEST MODE		
Output Voltage Open Circuit Limit)	Range:	3.00 – 8.00 VAC	
Output Fre- quency	Range:	60 or 50 Hz, User Selectable	
Output Current	Range: Resolution: Accuracy:	1.00 – 40.00 A 0.01 A ± (2% of setting + 0.02 A)	
Maximum Loading	1.00 – 10.00 A, 10.01 – 30.00 A 30.01 – 40.00 A	$_{\text{A}}$, $0-200~\text{m}\Omega$	
HI and LO-Limit	Range: Resolution: Accuracy:	$\begin{array}{l} 0-150 \ m\Omega \ for \ 30.01-40.00 \ A \\ 0-200 \ m\Omega \ for \ 10.01-30.00 \ A \\ 0-600 \ m\Omega \ for \ 1.00-10.00 \ A \\ 1 \ m\Omega \\ \pm (2\% \ of \ reading + 2 \ m\Omega) \end{array}$	
	Range: Resolution: Accuracy:	0 – 600 m Ω for 1.00 – 5.99 A 1 m Ω ± (3% of reading + 3 m Ω)	
Dwell Timer	Range:	0.5 – 999.9 sec (0=Continuous)	
Milliohm Offset	Range:	$0-200~\text{m}\Omega$	
CONTINUITY TE	ST MODE		
Output Current	DC 0.01 A ± 0.00001 A		
Resistance Display	Range:	$0.00-10000\Omega$	
HI and LO-Limit	Range: Resolution:	1: $0.00 - 10.00 \Omega$	
	Range 2: Resolution:	10.1 – 100.0 Ω 0.1 Ω	
	Range 3: Resolution: Accuracy:	101 – 1,000 Ω 1 Ω ± (1% of reading + 3 counts)	
	Range 4: Resolution: Accuracy:	1,001 – 10,000 Ω 1 Ω ± (1% of reading + 10 counts) (Max Limit: 0=OFF)	
Dwell Timer	Range:	0.0, 0.3 – 999.9 sec (0=Continuous)	
Milliohm Offset	Range:	0.00 – 10.00 Ω	
RUN TEST MODE	(Models 82)	X6 & 82X7 only)	
DUT Power	Voltage: Current: Range: Resolution: Accuracy:	16 AAC max continuous 0.0 – 277.0 VAC Full Scale 0.1 V	
Delay Time Setting	Range:	0.2 – 999.9 seconds	
Dwell Time	Range:	0.1 – 999.9 seconds (0=Continuous)	

OMNIA® II Series

RUN TEST MO	DE CONTINUE	D (Models 8	32X6 & 82X7 only)		
Trip Point	Voltage				
Settings & Metering	Volt-Hi Volt-LO	Range: Resolu- tion: Accuracy:	30.0 – 277.0 VAC 0.1 V ± (1.5% of setting + 0.2 V), 30.0–277 VAC		
	Current				
	Amp-HI Amp-LO	Range: Resolu- tion: Accuracy:	0.0 – 16.00 AAC 0.01 A ± (2.0% of setting + 2 counts)		
	Watts				
	Power-HI Power-LO	Range: Resolu- tion: Accuracy:	0 – 4,500 W 1 W ± (5.0% of setting + 3 counts)		
	Power Factor				
	PF-HI PF-LO	Range: Resolu- tion: Accuracy:	0.000 – 1.000 0.001 ± (8% of setting + 2 counts)		
	Leakage Curren	t			
	Leak-HI Leak-LO	Range: Resolu- tion: Accuracy:	0.00 – 10.00 mA (0=OFF) 0.01 mA ± (2% of setting + 2 counts)		
Timer Display	Range: Resolution: Accuracy:	ange: 0.0 – 999.9 seconds 0.1 second			
LEAKAGE CUF	RRENT TEST MO	DDE (Mode	ls 82X6 & 82X7 only)		
DUT Power	Voltage: Current:	0 – 277 VAC 16 AAC max			
	Voltage Display	Range: Resolu- tion: Accuracy:	0.0 – 277.0 VAC Full Scale 0.1 V ± (1.5% of reading +0.2 V), 30.0 – 277.0 VAC		
	Short Circuit Protection:	23 AAC, Res	sponse Time < 3 s		
Reverse Power Switch	Reverse polarity switch setting select ON/OFF/AUTO ON: Reverse power OFF: Normal AUTO: Automatic Reverse Polarity				
Neutral Switch	ON/OFF selectio	n for single fa	ult condition		
Ground Switch	ON/OFF selectio	n for Class I s	ingle fault condition		
Probe Setting	Surface to Line (F	Surface to Surface (PH – PL) Surface to Line (PH – L) Ground to Line (G – L)			
Touch Current High Limit (rms)	Range: Resolution:	0.0 μA ~ 999 0.1 μA / 1 μA	2.9 μΑ 1000 μΑ ~ 10.00 mA \ / 0.01 mA		

LEAKAGE CURF	RENT TEST MC	DDE CONTINUED (Models 82X6 & 82X7 only)	
Touch Current	Range 1:	0.0 μA ~ 32.0 μA, frequency DC, 15 Hz – 1 MHz	
Display (rms)	Range 2:	28.0 μA ~ 130.0 μA, frequency DC, 15 Hz – 1 MHz	
	Range 3:	120.0 μA ~ 550.0 μA, frequency DC, 15 Hz – 1 MHz	
	Resolution for Ranges 1, 2, 3:	0.1 μΑ	
	Accuracy for Ranges 1, 2, 3:	DC: 15 Hz < f <100 KHz: \pm (2% of reading + 3 counts) 100 KHz < f < 1 MHZ: \pm 5% of reading (10.0 μ A $-$ 999.9 μ A)	
	Range 4:	400 μA ~ 2100 μA, frequency DC, 15 Hz – 1 MHz	
	Range 5:	800 μA ~ 8500 μA, frequency DC, 15 Hz – 1 MHz	
	Resolution for Ranges 4 & 5:	1 μΑ	
	Accuracy for Ranges 4 & 5:	DC: 15 Hz < f <100 KHz: \pm (2% of reading + 3 counts) 100 KHz < f < 1 MHZ: \pm 5% of reading (10 μ A $-$ 8500 μ A)	
	Range 6:	8.00 mA ~ 10.00 mA, frequency DC 15 Hz – 100 kHz	
	Resolution:	0.01 mA	
	Accuracy:	DC: 15 Hz < f < 100 KHz: \pm 5% of reading (0.01 mA -10.00 mA)	
Touch Current	Range 1:	0.0 μA ~ 32.0 μA, frequency DC – 1 MHz	
Display (Peak)	Range 2:	28.0 μA ~ 130.0 μA, frequency DC – 1 MHz	
	Range 3:	120.0 μA ~ 550.0 μA, frequency DC – 1 MHz	
	Resolution for Ranges 1, 2, 3:	0.1 μΑ	
	Accuracy for Ranges 1, 2, 3:	DC: \pm (2% of reading + 2 μ A) 15 Hz < f < 1 MHZ : \pm 10% of reading + 2 μ A	
	Range 4:	400 μA ~ 2100 μA, frequency DC – 1 MHz	
	Range 5:	1800 A ~ 8500 μA, frequency DC – 1 MHz	
	Resolution for Ranges 4 & 5:	1 μΑ	
	Accuracy for Ranges 4 & 5:	DC: \pm (2% of reading + 2 μ A) 15 Hz < f < 1 MHz: \pm (10% of reading + 2 μ A)	
	Range 6:	8.0 mA ~10.00 mA, frequency DC – 100 KHz	
	Resolution:	0.01 mA	
	Accuracy:	DC: ± (2% of reading + 3 counts) 15 Hz < f < 100 KHz: ± (10% of reading + 2 counts)	
MD Circuit Module	MD1: UL544NP, UL484 , UL923, UL471, UL867, UL697 MD2: UL544P MD3: IEC 60601-1 MD4: UL1563 MD5: IEC60990 Fig4 U2, IEC62368-1, IEC60335-1, IEC60598-1, IEC60065, IEC61010 MD6: IEC60990 Fig5 U3, IEC60598-1 MD7: IEC62368-1, IEC61010-1 FigA.2 (2K ohm) for Run function MD8: IEC60990/IEC62368-1 Fig4 U1		
External MD	Basic measuring element 1 $k\Omega$		
Scope Output Interface	BNC type connector on rear panel for Oscilloscope connection		

AC POWER SO	OURCE (82X7	only)		
Output	Power:	630 VA and 500	W Maximum	
	Voltage:	0 – 150.0 V / 0 –	277.0 V	
	Current:	4.20 A maximum for 0 – 150 V range 2.10 A maximum 0 – 277 V range		
	Distortion:	\leq 1% at 45-500 Hz and output voltage within the $$ 80 $^{\sim}$ 140 VAC at Low Range or the 160 $^{\sim}$ 277 VAC at High Range (Resistive Load)		
	Regulation:	$\leq 0.5\% + 5$ V (resistive load), from no load to full load and Low Line to High Line (combined regulation)		
	Crest Factor:	>3		
	Test Timing:	< 350 ms at start and between		
	Limit:	Steps when inte	rnal AC source is ON	
Settings	Voltage	Low Range:	0.0 – 150.0 V	
		High Range:	0.0 – 277.0 V	
		Resolution:	0.1 V	
		Accuracy:	± (1.5% of setting + 2 counts)	
	Frequency	Range: Resolution: Accuracy:	45.0 Hz – 99.9 Hz 0.1 Hz ± 0.1% of setting	
		Range: Resolution: Accuracy:	100 Hz – 500 Hz 1 Hz ± 0.1% of setting	
	A-HI-Limit	Range: Resolution: Accuracy:	4.20 A / 2.10 A 0.01 A ± (2% of reading + 2 counts)	
Measurement	Voltage	Range: Resolution: Accuracy:	0.0 – 277.0 V 0.1 V ± (1.5% of reading + 2 counts)	
			0.00 – 16.00 A 0.01 A ± (2% of reading + 2 counts)	
		Power: Resolution: Accuracy:	0 - 4500 1 $\pm (5\% \text{ of reading} + 3 \text{ counts}) \text{ for PF} > 0.100$	
		Power Factor: Resolution: Accuracy:	0.000 – 1.000 0.001 ± (8% of reading + 5 counts)	
		Frequency: Resolution: Accuracy:	45 – 500 Hz 0.1 Hz ± 0.1 Hz	

GENERAL SPECIFICATIONS		
PLC Remote Control	Input: Test, Reset, Interlock, Recall File 1 through 3 Output: Pass, Fail, Test-in-Process	
Safety	Built-in SmartGFI circuit	
Memory	10,000 Steps	
Interface	Standard: USB/RS-232 Optional: Ethernet or GPIB	
Security	Advanced security system with access levels and username/password requirements	
Dimensions (W x H x D)	16.93" x 5.24" x 19.69" (430 x 133 x 500 mm)	
Weight	8204: 82 lbs (37 kg) 8254: 92 lbs (42 kg) 8206/8207: 83 lbs (38 kg) 8256/8257: 103 lbs (47 kg)	

Why We Use Counts
Associated Research publishes some specifications using "counts" which allows us to provide a better indication of the instrument's capabilities across measurement ranges.
A count refers to the lowest resolution of the display for a given measurement range. For example, if the resolution for voltage is 1V then 2 counts = 2 V.

The default of the Adapter Box accesscoy come in L-N polarity. N-L polarity is available

Specifications subject to change without notice.



Our HYAMP® Series provides manufacturers with data-driven results and greater test flexibility required in today's complex test environment. Quickly collect test data and test settings from the convenient front panel USB port onto a standard USB flash drive. Use the front panel barcode connection to associate products with preprogrammed test files. Test with greater flexibility by performing either AC Ground Bond or DC Ground Bond at a maximum of 40 A of current. The HYAMP® features a drastically reduced weight and footprint making it the ideal lightweight Ground Bond solution for laboratory and production line testing applications. Easily interconnect with the Hypot® Series to form a complete safety compliance system.



Find the Model that Fits Your Testing Needs



3240 AC/DC

SAFETY & PRODUCTIVITY **FEATURES**







PLC Remote Basic PLC relay control

Interlock Easily disable HV output

Remote Safety

Data Transfer Easily import/ export test files and data via USB



Barcode Capability Direct barcode



Multiple Languages Multi-Language user interface



Ground Bond Voltage Drop Monitor voltage drop vs resistance



FailCHEK™ Confirms failure detection



Prompt & Hold Provides alerts between tests



Advanced User Security Customize ID & password protection



Accredited Accredited options



4-Wire Measurement More accurate measurement



Interconnection Interconnect with Hypot® to form a complete test system



On Board Data Storage Save up to 1.500 Test

Results on-



WithStand® Software

INPUT SPECIFICATION	ONS	
Voltage	100 – 120 VAC / 200 – 240 VAC ± 10% Auto Range	
Frequency	50/60Hz ± 5%	
Fuse	10 A, Slow B	low 250 VAC
GROUND BOND TE	ST MODE	
Output Voltage (Open Circuit Voltage)	Range: Resolution: Accuracy:	3.00 – 8.00 VAC/DC 0.01 VAC/DC ± (3% of setting + 3 counts)
Output Frequency	50 or 60 Hz,	User Selectable/DC
Output Current	Range: Resolution: Accuracy:	0 – 150 mΩ for 30.01 – 40.00 A 0 – 200 mΩ for 10.01 – 30.00 A 0 – 600 mΩ for 1.00 – 10.01 A 0.1 A ± (3% of setting + 3 counts)
Maximum Loading	Range: Resolution: Accuracy:	1.00 - 10.00 A, $0 - 600$ mΩ $10.01 - 30.00$ A, $0 - 200$ mΩ $10.01 - 40.00$ A, $0 - 150$ mΩ 10.01 mΩ 1
HI and LO-Limit Resistance	Range: Resolution: Accuracy:	$ 0 - 150 \ m\Omega \ for \ 30.01 - 40.00 \ A $ $ 0 - 200 \ m\Omega \ for \ 10.01 - 30.00 \ A $ $ 0 - 600 \ m\Omega \ for \ 1.00 - 10.01 \ A $ $ 1 \ m\Omega $ $ \pm (2\% \ of \ setting + 2 \ counts) $
HI and LO-Limit Voltage	Range: Resolution: Accuracy:	0.00 – 6.00 V 0.01 ± (2% of settings + 2 counts)
Dwell Time Setting	Range:	0, 0.5 – 999.9 sec (0=Continuous)
Ω Offset Capability	Range: Resolution: Accuracy:	0 – 100 mΩ 1 mΩ ± (2% of setting + 2 counts)
V Offset Capability	Range: Resolution: Accuracy:	0.00 – 4.00 V 0.01 V ± (2% of setting + 2 counts)
Current Display	Range: Resolution: Accuracy:	0.00 – 40.00 AAC/DC 0.01 AC/DC ± (3% of reading + 1 count)
Voltage Display	Range: Resolution: Accuracy:	0.00 – 8.00 VAC/DC 0.01 AC/DC ± (2% of reading + 2 counts)
Ohmmeter Display	Range: Resolution: Accuracy:	0 – 600 mΩ for 1.00 – 5.99 A 1 mΩ $\pm (3\% \text{ of reading } + 3 \text{ counts})$
	Range: Resolution: Accuracy:	$0-600$ m Ω for $6-40$ A 1 m Ω \pm (2% of reading + 2 counts)

GENERAL SPECIFICATIO	GENERAL SPECIFICATIONS		
Remote Control and Signal I/O	The following input and output signals are provided through two 9 pin D type connectors: Inputs: Test, Reset, Hardware Interlock, File Recall Outputs: Pass, Fail, Test-in-Process, Reset-Out, Start-Out Hardware Interlock (safety)		
Memories	50 steps 1500 test results		
Interface	USB standard		
Language	English, Traditional Chinese, Simplified Chinese, Turkish, Portuguese, Spanish, German, French		
Security	Multiple user setups with ID and password		
Dimensions (W x H x D)	8.5" x 3.5" x 11.9" (215 x 88.1 x 300 mm)		
Weight	11 lbs (5 kg)		

Why We Use Counts

Associated Research publishes some specifications using "counts" which allows us to provide a better indication of the instrument's capabilities across measurement ranges. A count refers to the lowest resolution of the display for a given measurement range. For example, if the resolution for voltage is 1V then 2 counts = 2 V.

Specifications subject to change without notice.



Our HypotMAX® Series is a complete line of automated Hipot instruments designed to meet the demanding requirements of high voltage applications. We've included our patented SmartGFI® feature for maximum operator safety as well as a variety of advanced features to increase productivity on the production line and in the lab. Set up and run tests with confidence from our intuitive user interface or automate with a PC.



AVAILABLE INTERFACES







SAFETY & PRODUCTIVITY **FEATURES**







PLC Remote Basic PLC relay control

Automatic operator shock protection

Interlock Easily disable HV output









Arc Detection High frequency detection

Reduce ramp time during DC Hipot

Charge-LO® Confirms proper DUT connection





Accredited Accredited calibration options

available

WithStand® Automation Software

Find the Model that Fits Your Testing Needs





7705	•	
7710		•
7715	•	
7720		•

INPUT SPECIFICATIONS		
Voltage	115/230 VAC ± 10%, Single Phase, User Selection	
Frequency	50/60 Hz ± 5%	
Fuse	6.3 A, 250 V Slow Blow	

Frequency	50/60 Hz ± 5%			
Fuse	6.3 A, 250 V Slow Blow			
DIELECTRIC WITHSTAND TEST MODE				
Output Rating	7705: 7710: 7715: 7720:	10 kV @ 20 mA 12 kV @ 10 mA 20 kV @ 10 mA 20 kV @ 5 mA	NDC NAC	
HI-Limit and LO-Limit	7705	Range 1: Resolution: Range 2: Resolution:	0.0 – 9.999 mA 0.001 mA 10.00 – 20.00 mA 0.01 mA	
	7710	Range 1: Resolution: Range 2: Resolution:	0.00 – 999.9 μA 0.1 uA 1,000 – 9,999 μA 1 μA	
	7715	Range: Resolution:	0.00 – 9.999 mA 0.001 mA	
	7720	Range 1: Resolution: Range 2: Resolution:	0.0 – 999.9 μA 0.1 μA 1,000 – 5,000 μA 1 μA/step	
	77XX	Accuracy:	± (2% of setting + 2 counts)	
DC Ramp HI	7710	13 mA peak m	aximum, 10 mADC, ON/OFF selectable	
	7720	6.75 mA peak	maximum, 5 mADC, ON/OFF selectable	
DC Charge LO	7710/7720	Range:	$0.0 - 350 \mu\text{ADC}$ or auto set	
Arc Detection	7705		: voltage < 7.00 kV : voltage ≥ 7.00 kV	
	7710/7720	1 – 9		
	7715		voltage < 15.00 kV voltage ≥ 15.00 kV	
Voltage Display	7705	Range: Accuracy:	0.00 – 10.00 kV Full scale ± (1.5% of reading + 20 V)	
	7710	Range: Accuracy:	0.00 – 12.00 kV Full scale ± (2% of reading + 20 V)	
	7715/7720	Range: Accuracy:	0.00 – 20.00 kV Full scale ± (1.5% of reading + 20 V)	
Current Display	7705	Auto Range Range 1: Range 2:	0.000 – 3.500 mA 3.00 – 20.00 mA	
	7710	Auto Range Range 1: Range 2: Range 3:	0.0 – 350.0 μA 300 – 3500 μA 3,000 – 9,999 μA	
	7715	Auto Range Range 1: Range 2:	0.000 – 3.500 mA 3.00 – 10.00 mA	
	7720	Auto Range Range 1: Range 2:	0.0 – 350.0 μA 300 – 5,000 μA	
DC Output Ripple	7710	< 5% Ripple at	t 12 kV @ 9,999 μA, Resistive Load	
	7720	< 5% Ripple at	20 kV @ 4,999 μA, Resistive Load	
AC Output Waveform	Sine Wave, 0	Crest Factor = 1	.3 – 1.5	
Output Frequency	Range:	50/60 Hz, User ± (1% of outpu No load to full	ıt + 5 V) from Regulation	
Output Regu- lation	± (1% of out	\pm (1% of output + 10 V) from no load to full load		
Discharge Timer	7710	No load < 400	ms	
	7720	No load < 500	ms	
Dwell Timer		Range: AC Range: DC Range:	0, 0.3 – 999.9 sec (0=Continuous) 0, 0.3 – 999.9 sec or min (0=Continuous) 0, 0.4 – 999.9 sec or min (0=Continuous)	
Ramp Timer	7705/7715	Range:	0.3 – 999.9 sec	
	7710/7720	Range:	0.4 – 999.9 sec	
Ground Conti- nuity	Max. Ground	Max. Ground Resistance 1 Ω ± 0.1 Ω , fixed		

DIELECTRIC WITHSTAND TEST MODE			
Ground Fault Interrupt	HV Shut Down Speed < 1 ms GFI Trip Current 1 mA max		
GENERAL SPECIFICATIONS			
Memory	50 memories w/ 8 steps per memory		
Mechanical	Tilt-up front feet		
Interface	Standard: USB, RS-232 Optional: GPIB		
Dimensions (W x H x D)	16.93" x 5.24" x 15.75" (430 x 133 x 400 mm)		
Weight	7705: 63.3 lb (28.7kg) 7710: 63.1 lb (28.6kg) 7715: 59.4 lb (26.9kg) 7720: 61.6 lb (27.9 kg)		


Why We Use Counts

Associated Research publishes some specifications using "counts" which allows us to provide a better indication of the instrument's capabilities across measurement ranges. A count refers to the lowest resolution of the display for a given measurement range. For example, if the resolution for voltage is 1V then 2 counts = 2 V.


 ${\bf Specifications\ subject\ to\ change\ without\ notice.}$



Our patented SC6540 multiplexer pioneered the largest productivity improvement in the electrical safety compliance industry in years. With up to 16 independent high voltage or high current channels in a convenient 2U design, the SC6540 can be customized in 10 different configurations for multi-point Hipot, Ground Bond, Insulation Resistance, and Leakage Current testing. Configure the SC6540 according to your needs, and interface with your OMNIA® II, HypotULTRA® or LINECHEK® II instrument to improve production line throughput or expand lab testing capability. Operate from the front panel of your AR instrument or utilize a variety of automation interfaces for direct PC control.

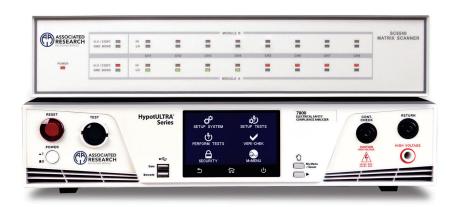

Find the Model that Fits Your Testing Needs

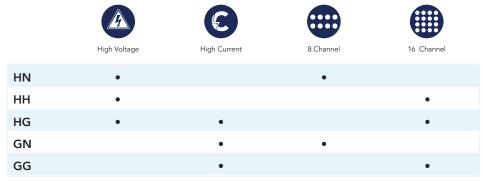

Available in both main and secondary configurations

AVAILABLE INTERFACES









PRODUCTIVITY ENHANCING FEATURES



LINECHEK® II to form a complete test system





FOR USE WITH THE **FOLLOWING TESTS**













MODULAR MULT	IPLEXER SP	ECIFICATIONS		
Input (Main only)	115 VAC (± 10%), 50/60 Hz, single phase 230 VAC (± 10%), 50/60 Hz, single phase User selectable			
Fuse (Main only)	250 V/2 A/fa	st-blow		
PC Control (Main only)	Standard: US Optional: Eth			
Multiplexer Control	aries	Main: One Multiplexer bus output controls, up to 4 additional secondaries Secondary: One output and one input		
Maximum HV Rating	5 kV AC and	5 kV AC and DC		
Maximum HC Rating	40 A			
Number of Possible Channels	8 or 16			
HV Output	100' reel HV cable rated for up to 30 kV Terminations with 8 HV connectors			
GND Output	20 terminals provided, to accept 10/12 AWG Terminations hook-up wire (user supplied wire)			
Temperature	32° – 104° F (0° – 40° C)			
Humidity	0 – 80%			
Altitude	6,560 ft. (2,000 m)			
Mechanical	2U with tilt-up front feet			
Dimensions (W x H x D)	17" x 4.07" x 12.96" (432 x 103 x 329 mm)			
Weight	Main: 20.05 lbs. max. (9.09 kg) (with 2 high voltage modules) 15.45 lbs. max. (7.01 kg) (with 2 high voltage modules)			

CONFIGURATIONS

The modular design can be customize to fit your application. In addition to main or secondary control, the SC6540 can be set up in the following configurations: 8 or 16 high voltage channels, 8 or 16 high current channels, and 8 high voltage channels and/or 8 high current channels. Refer to the images for details.

The different configurations (shown below) are indicated by the following alpha designators

M – Main Multiplexer

H - 8 High Voltage Channels

HH – 16 High Voltage Channels

G – 8 Ground Bond Channels GG – 16 Ground Bond Channels

N – Empty Module S – Secondary



MODEL SC6540 HNM*

8 Channel High Voltage Multiplexer



MODEL SC6540 HHM*

16 Channel High Voltage Multiplexer



MODEL SC6540 HGM*

8 Channel High Voltage Multiplexer 8 Channel High Current Multiplexer



MODEL SC6540 GNM*

8 Channel High Current Multiplexer



MODEL SC6540 GGM*

16 Channel High Current Multiplexer

*Also available in secondary configuration



Our LINECHEK® II model 620L provides 7 measuring devices (MD's) compliant with international certification bodies as well as a convenient switching network to simulate all 8 required fault conditions, everything you need for full Leakage Current compliance. Utilize the intuitive user interface or control via a PC for more advanced automated applications that require data storage and analysis. The 620L handles up to 40 A of continuous current and can be interfaced to an SC6540 modular multiplexer for multi-point testing. Interconnect the 620L to an OMNIA® II instrument to form a complete electrical safety compliance testing system.



AVAILABLE INTERFACES









SAFETY & PRODUCTIVITY FEATURES







Prompt & Hold Interlock Provides alerts & instructions

Remote Safety Easily disable HV output

Active Link Continuous power during test steps







PLC Remote Basic PLC

Multiplexer with SC6540

Interconnection Interconnect with OMNIA® II or HypotUL-TRA® to form a complete test system





Cal-Alert® alerts for calibration

Automation Software

Find the Model that Fits Your Testing Needs







620L

20

INPUT SPECIFICA	ATIONS					
Voltage	115/230 VA	115/230 VAC ± 10%, User Selection				
Frequency	50/60 Hz ± 5	5%				
Fuse	2 A Slow Blo	ow 250 VAC				
LINE CONDITION	NS					
Reverse Power		ower polarity reversal				
Switch	· ·					
Neutral Switch	Neutral swit	ch on/off selection for single fault				
Ground Switch		tch on/off selection for class I single fault				
PROBE SETTING	S					
Surface to Surface	(PH – PL)					
Surface to Line	(PH – L)					
Ground to Line	(G – L)					
LEAKAGE LIMIT	SETTINGS					
Touch Current High/Low Limit (rms)	Range: Resolu- tion:	0.0 μA – 999.9 μA / 1,000 μA – 9,999 μA / 10.00 mA – 20.00 mA 0.1 μA / 1 μA / 0.01 mA				
Touch Current	Range:	0.0 μA -999.9 μA / 1,000 uA – 9,999 μA / 10.00 mA – 30.00				
High/Low Limit (Peak)	Resolu- tion:	mA 0.1 μA / 1 μA / 0.01 mA				
DISPLAY						
Touch Current	Range:	0.0 μA – 550 μA, frequency DC, 15 Hz – 1 MHz				
Display (rms)	Resolu- tion: Accuracy:	0.1 µA DC: 15 Hz ≤ f ≤ 100 kHz: ± (2% of reading + 3 counts) 100 kHz ≤ f ≤ 1 MHz: ± 5% of reading (10.0 µA – 999.9 µA)				
	Range: Resolu- tion:	400 μA – 8,500 μA, frequency DC, 15 Hz – 1 MHz 1 μA DC: 15 Hz \leq f \leq 100 kHz: \pm (2% of reading + 3 counts) 100 kHz \leq f \leq 1 MHz: \pm 5% of reading, (10.0 μA – 8,500 μA)				
	Range: Resolution: Accuracy:	8.00 mA – 20.00 mA, frequency DC, 15 Hz – 100 KHz 0.01 mA DC: 15 Hz ≤ f ≤ 100 MHz: ± 5% of reading (0.01 mA – 20.00 mA)				
Touch Current Display (peak)	Range: Resolu- tion: Accuracy:	0.0 µA − 550 µA, frequency DC − 1 MHz 0.1 µA ± (2% of reading + 2 µA) 15 Hz ≤ f ≤ 1 MHz, ± 10% of reading + 2 µA				
	Range: Resolu- tion: Accuracy:	400 μA − 8,500 μA, frequency DC − 1 MHz 1 μA ± (2% of reading + 2 μA) 15 Hz ≤ f ≤ 1 MHz, ± 10% of reading + 2 μA				
	Range: Resolu- tion: Accuracy:	8.00 mA $-$ 30.00 mA, frequency DC $-$ 100 kHz 0.01 mA \pm (2% of reading + 3 counts) 15 Hz \leq f \leq 100 kHz, \pm 10% of reading + 2 counts				
MEASURING DE	VICE MODU	JLE				
MD1	UL544NP, U	L484 , UL923, UL471, UL867, UL697				
MD2	UL544P					
MD3	IEC 60601-1					
MD4	UL1563					
MD5	IEC60990 Fig4 U2, IEC62368-1, IEC60335-1, IEC60598-1, IEC60065, IEC61010					
MD6	IEC60990 Fig5 U3, IEC60598-1					
MD7	IEC62368-1, IEC61010-1 FigA.2 (2 kohm) for Run function					
External MD	Basic measuring element 1 kohm					
MD Voltage Limit	70 VDC					

DUT POWER						
AC Voltage	0.0 – 277.0 V	0.0 – 277.0 V				
AC Current	40 A max co	ntinuous				
AC Voltage High/Low Limit	Range: Resolu- tion:	0.0 – 277.0 V 0.1 V/step				
AC Voltage Display	Range: Resolu- tion: Accuracy:	0.0 – 277.0 V 0.1 V/step ± (1.5% of reading + 2 counts), 30.0 – 277.0 V				
Delay Time Setting	Range: Resolu- tion:	0.5 – 999.9 sec 0.1 sec				
Dwell Time Setting	Range: Resolu- tion: Accuracy:	0, 0.5 – 999.9 sec (0=Continuous) 0.1 sec ± (0.1% of reading + 0.05 seconds)				
Failure Protection	On Start-Up – Neutral Voltage Check (Neutral – V) Over current and ground current check (Line – OC)					

GENERAL SPECIFICATIONS				
Memory	50 Memories, 30 steps per each memory File locations can link 900 steps max			
Mechanical	Bench or rackmount with tilt-up feet			
Interface	Standard: USB, RS-232 Optional: Ethernet, GPIB			
Dimensions (W x H x D)	16.93" x 5.24" x 11.81" (430 x 133 x 300 mm)			
Weight	26.45 lbs (12 kg)			

Why We Use Counts

Associated Research publishes some specifications using "counts" which allows us to provide a better indication of the instrument's capabilities across measurement ranges. A count refers to the lowest resolution of the display for a given measurement range. For example, if the resolution for voltage is 1V then 2 counts = 2 V.

The default of the Adapter Box accesscoy come in L-N polarity. N-L polarity is available upon request.

Specifications subject to change without notice.

MedTEST A Complete Electrical Safety Testing

System that Satisfies the Most Demanding **Medical Compliance Requirements**





AVAILABLE INTERFACES









GPIB

Our MedTEST system can be designed to provide a complete test solution for medical device manufacturers need in conforming to IEC 60601-1 3rd Edition Standard. Customize your MedTEST system to satisfy your individual testing requirements including Hipot, Ground Bond, Insulation Resistance, Functional Run and leakage current testing for all B, BF and CF type applied parts including Mains on Applied Parts (MOAP) tests. Up to 40 A of continuous DUT current combined with our Active Link® technology reduces overall test time and integration with our modular multiplexer SC6540 allows for multi-point sequential testing without the need to change test leads. Get the most from your test system by utilizing our WithStand® software for maximum productivity-enhancing benefits.



Rack cabinet shown in image is for illustration only. Ikonix does not sell or distribute the rack cabinet.

SAFETY & PRODUCTIVITY FEATURES



operator shock

protection





Remote Safety



Easily disable HV output

Prompt & Hold Provides alerts & instructions between tests



Multiple . Languages Multi-Language user



Active Link® Continuous test steps



Mv Menu Customize your own shortcut menu



DualCHEK® Simultaneous Hipot and Ground Bond



Multiplexer Available with optional HV



Multiplexer Compatible with SC6540



FailCHFK™ Confirms detection



Cal-Alert® Tracks and alerts for calibration



Reduce ramp time during DC Hipot







Accredited Accredited calibration options available



WithStand® Automation Software









Continuity







Run



Resistance

Visit Us Online ikonixasia.com

POPULAR MEDTEST CONFIGURATIONS



OMNIA® II 8207 AND SC6540

- All-in-one testing system (Hipot, Ground Bond, Insulation Resistance, and Leakage Current)
- Built in 500 VA AC power source
- Efficient use of rack space
- SC6540 provides automated multi-point testing
 Most common applications incorporate 8 or 16 port multiplexers



OMNIA® II 8206, SC6540 AND POWERED BY AN OCCUPANIONIX BRAND AC POWER SOURCE

- All-in-one testing system (Hipot, Ground Bond, Insulation Resistance, and Leakage Current)
- Compatible EEC power source provides power to DUT*
- SC6540 provides automated multi-point testing.
 Most common applications incorporate 8 or 16 port multiplexers
 *Choose from EEC 8500 Series.



OMNIA® II 8204, 620L, SC6540 AND POWERED BY AN COLOR AC POWER SOURCE

- All-in-one testing system (Hipot, Ground Bond, Insulation Resistance, and Leakage Current)
- Compatible EEC power source provides power to DUT*
- SC6540 provides automated multi-point testing
 Most common applications incorporate 8 or 16 port multiplexers
- Up to 40 A continuous current capability for applications that draw greater than 16 A of current

*Choose from EEC 8500 Series.

MedTEST

LINE CONDITION	NS						
Reverse Power Switch	Switch for p	Switch for power polarity reversal					
Neutral Switch	Neutral switch on/off selection for single fault						
Ground Switch	Ground swit	Ground switch on/off selection for class I single fault					
PROBE SETTING	S						
Surface to Surface	(PH – PL)						
Surface to Line	(PH – L)						
Ground to Line	(G – L)						
LEAKAGE LIMIT	SETTINGS						
Touch Current High/Low Limit (rms)	Range: Resolu- tion:	0.0 μA – 999.9 μA / 1,000 μA – 9,999 μA / 10.00 mA – 20.00 mA 0.1 μA / 1 μA / 0.01 mA					
Touch Current High/Low Limit (Peak)	Range: Resolu- tion:	0.0 μA -999.9 μA / 1,000 uA - 9,999 μA / 10.00 mA - 30.00 mA mA 0.1 μA / 1 μA / 0.01 mA					
MEASURING DE	VICE MODU	JLE					
MD1	UL544NP, U	L484 , UL923, UL471, UL867, UL697					
MD2	UL544P						
MD3	IEC 60601-1						
MD4	UL1563						
MD5	IEC60990 Fig4 U2, IEC62368, IEC60335-1, IEC60598-1,IEC60065, IEC61010						
MD6	IEC60990 Fig5 U3, IEC60598-1						
MD7	IEC62368, IEC61010-1 FigA.2 (2 kohm) for Run function						
External MD	Basic measuring element 1 kohm						
MD Voltage Limit	70 VDC						
DUT POWER							
AC Voltage	0.0 – 277.0 V	,					
AC Current	40 A max co	ntinuous					
AC Voltage High/Low Limit	Range: Resolu- tion:	0.0 – 277.0 V 0.1 V/step					
AC Voltage Display	Range: 0.0 – 277.0 V Resolution: ± (1.5% of reading + 2 counts), 30.0 – 277.0 V Accuracy:						
Delay Time Setting	Range: Resolu- tion:	Range: 0.5 – 999.9 sec Resolu- 0.1 sec					
Dwell Time Setting	Range: Resolu- tion: Accuracy:	0, 0.5 – 999.9 sec (0=Continuous) 0.1 sec ± (0.1% of reading + 0.05 seconds)					
Failure Protection		– Neutral Voltage Check (Neutral – V) t and ground current check (Line – OC)					

DIELECTRIC WITI	HSTAND TES	T MODE			
Output Rating*	5 kV @ 50 mAAC 6 kV @ 20 mADC				
Voltage Setting	Range: Resolution: Accuracy:	0 – 5,000 VAC, 0 – 6,000 VDC 1 V ± (1.5% of setting + 5 V)			
HI and LO-Limit	AC Total	Range: Resolution: Accuracy:	0.000-9.999 mA 0.001 mA ± (2% of setting + 2 counts)		
		Range: Resolution: Accuracy:	10.00 – 50.00 mA 0.01 mA ± (2% of Setting + 2 counts)		
	AC Real	Range: Resolution: Accuracy:	0.000 - 9.999 mA 0.001 mA $\pm (3\% \text{ of setting} + 50 \mu\text{A})$		
		Range: Resolution: Accuracy:	10.00 - 50.00 mA 0.01 mA $\pm (3\% \text{ of setting} + 50 \mu\text{A})$		
	DC	Range: Resolution: Accuracy:	$0.00 - 999.9 \mu\text{A}$ $0.1 \mu\text{A}$ $\pm (2\% \text{ of setting} + 2 \text{ counts})$		
		Range: Resolution: Accuracy:	1,000 – 20,000 μ A 1 μ A ± (2% of setting + 2 counts)		
Ramp HI	> 20 mA peak maximum, ON/OFF selectable				
Charge LO	Range: 0.000 – 350.0 μA or Auto Set				
DC Output Ripple	≤ 4% Ripple rms at 5 kVDC @ 20 mA, Resistive Load				
Discharge Timer	< 50 msec for no load, < 100 msec for capacitor load (All capacitance values in MAX load spec below)				
Maximum Capacitive Load	$\begin{array}{lll} 1 \ \mu F < 1 \ kV & 0.08 \ \mu F < 4 \ kV \\ 0.75 \ \mu F < 2 \ kV & 0.04 \ \mu F < 6 \ kV \\ 0.50 \ \mu F < 3 \ kV & \end{array}$				
Output Frequency	50/60 Hz ± 0.1	1% , User Selection	n, 400/800 Hz Option		
AC Output Waveform	Sine Wave, Crest Factor = 1.3 – 1.5				
Output Regu- lation	\pm (1% of output + 5 V) from no load to full load and over input voltage range				
Dwell Timer	AC 0, 0.4 – 999.9 sec (0=Continuous) DC 0, 0.3 – 999.9 sec (0=Continuous)				
Ramp Timer	Ramp-Up AC: 0.1 – 999.9 Ramp-Down AC: 0.0-999.9 Ramp-Up DC: 0.4 – 999.9 Ramp-Down DC: 0.0, 1.0-999.9				
Ground Conti- nuity		0.1 A \pm 0.01 A, fixe Resistance: 1 Ω \pm			
Ground Fault Interrupt		GFI Trip Current: 5.0 mA max HV Shut Down Speed: < 1 ms			

^{*}Output voltage limited to 3.5 kV with 620L option 03 $\,$

CONTINUITY TES	ST MODE				
Output Current	DC 0.1 A ± 0.00001 A				
Resistance Display	Range: 0.00 – 10,000.00 Ω				
HI and LO-Limit	0.00 – 10,000	Ω			
Dwell Timer	Range: 0.0, 0.3 – 999.9 sec (0=Continuous)				
Milliohm Offset	Range:	0.00 – 10.00 Ω			
GROUND BOND	TEST MODE				
Output Voltage	Range:	3.00 – 8.00 VAC			
Output Frequency	50/60 Hz ± 0.1	%, User Selection			
Output Current	Range: Resolution: Accuracy:	1.00 – 40.00 A 0.01 A ± (2 % of setting + 2 counts)			
Output Regu- lation	± (1% of output voltage range	ut + 0.02 A) Within maximum load limits, and over input			
Maximum Loading	1.00 - 10.00 A, $0 - 600$ mΩ $10.01 - 30.00$ A, $0 - 200$ mΩ $10.01 - 40.00$ A, $0 - 150$ mΩ				
HI and LO-Limit	Range:	0 – 150 for 30.01 – 40.00 A			
	Range:	0 – 200 for 10.01 – 30.00 A			
	Range:	0 – 600 for 6.00 – 10.00 A			
	Range:	0 – 600 for 5.99 – 1.00 A			
	Resolution:	Resolution: $1 \text{ m}\Omega$			
	Accuracy:	6.00 – 40.00 A, ± (2% of setting + 2 Counts) 1.00 – 5.99 A, ± (3% of setting + 3 Counts)			
Milliohm Offset	Range:	$0-200~\text{m}\Omega$			
INSULATION RES	ISTANCE TE	ST MODE			
Output Voltage	Range:	30 – 1,000 VDC			
Charging Current	Maximum > 2	0 mA peak			
HI and LO-Limit	Range: Resolution:	0.05-99.99 MΩ 0.01 MΩ			
	Range: Resolution:	100.0 – 999.9 MΩ 0.1 MΩ			
	Range: Resolution:	1000 – 50,000 MΩ 1 MΩ			
Charge-LO	0.000 – 3.500	μA or Auto Set			
Ramp Timer	Ramp Up: Ramp Down:	0.1 – 999.9 secs 0.0, 1.0 – 999.9 secs			
Dwell Timer	0, 0.5 – 999.9	(0=Continuous)			
Delay Timer	0.5 – 999.9 secs				
Ground Fault Interrupt	GFI Trip Current: 5.0 mA max HV Shut down Speed: < 1 ms				

GENERAL SPECI	GENERAL SPECIFICATIONS				
Interface	Standard: USB, RS-232 Optional: Ethernet, GPIB				
Safety	Built-in SmartGFI® circuit				
Memory	620L: 50 memories, 30 steps per memory OMNIA® II: 10,000 steps				
AC POWER SOU	RCE				
AC Power Source	Up-to 6 kVA compatible power sources available				
Configuration	AC Power Source configuration depends on application. MedTEST hardware is configured for testing products with one side of the supply mains at earth potential (Fig 10 UL60601-1). MedTEST hardware is configured for unbalanced 0-277 V DUT input power. Custom Configurations available. Contact us for details.				

Why We Use Counts
Associated Research publishes some specifications using "counts" which allows us to provide a better indication of the instrument's capabilities across measurement ranges. A count refers to the lowest resolution of the display for a given measurement range. For example, if the resolution for voltage is 1V then 2 counts = 2 V.

Specifications subject to change without notice.




Interconnect our Hypot® Series Hipot Instrument with our HYAMP® Series Ground Bond instrument to form a complete safety compliance system. Easily operate both instruments from a single point of control on the production line or in a rack. All test systems are safety agency listed, include interconnect cables, and detailed directions on effortlessly interconnecting your system.

	Hypot® 3805	Hypot® 3855	Hypot® 3865	Hypot® 3870
	AC Hipot	AC Insulation Hipot Resistance	AC DC Hipot Hipot	AC DC Insulation Hipot Hipot Resistance
HYAMP® 3240 40A Ground Bond	System 32-05	System 32-55	System 32-65	System 32-70

SETTING UP A SAFE WORKSTATION

Setting up a safe and secure workstation is one of the best ways to protect your test operators. You can setup test stations with or without direct protection depending on your requirements.

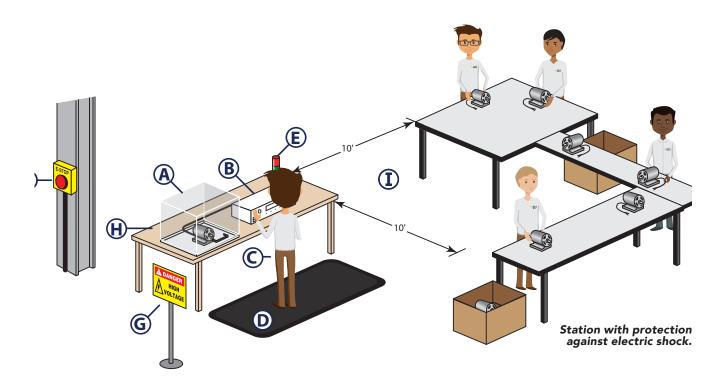

	Description
А	DUT Safety Enclosure - This is wired to the Hipot tester's Remote Safety Interlock. This protects you from touching the DUT while a test is in progress. When you open the enclosure door, it will immediately disable the instrument's high voltage output.
В	Hipot Tester – Performs test on the DUT
С	Test Operator
D	High Voltage Insulation Mat – This isolates you from ground which provides an additional means of protection when operating high voltage equipment.
E	Signal Tower Light – Gives an indication as to the status of the testing area. A green light indicates the Hipot instrument is not outputting high voltage and the test area is safe. A red light indicates that the Hipot instrument is active and to stay clear of the test area.
F	Emergency Stop Button – An E-stop button is located on the perimeter of the test area. In the event of an emergency, someone outside the test area can hit the E-Stop button to immediately cut off power to the entire test station.
G	Warning Signs – Mark the testing area with clearly posted signs that read: DANGER-HIGH VOLTAGE TEST AREA. AUTHORIZED PERSONNEL ONLY.
Н	Non-Conductive Work Bench – Only use a work bench made of non-conductive material such as plastic or wood. This ensures no stray leakage current could flow through you during a test.
I	NEC (National Electric Code) and NFPA (National Fire Protection Agency) stipulate that any unqualified workers shall not come within 10 feet of an EXPOSED energized circuit.

ESSENTIAL WORKSTATION PPE & ACCESSORIES

Class 3 Insulation Mat 40396

Thickness: 3/8" (9.53 mm)

Dimensions: 3' x 3' (91.44 x 91.44 cm)



High Voltage Warning Sign 39538



DUT Enclosure Wood Frame with Foam Interior 39067

Protect your operator from electric shock by enclosing your DUT. Our enclosures automatically disable the instrument's output when the enclosure door is opened. Our DUT Enclosures are designed to protect the operator from electric shock during testing. Interface an enclosure with our Remote Safety Interlock feature to automatically disable the instrument's output when the enclosure door is opened.

Outside dimensions (W x D x H): 24" x 19" x 11.5" (610 x 483 x 293 mm) Inside dimensions (W x D x H):20" x 16" x 10" (508 x 407 x 254 mm) 3/4" Walls, 3/4" Flame Retardant Foam, 1/4" Plexiglass cover



Dual Palm Remote Switch

DPR-01

Prevent your operator from touching a DUT as their hands must stay on the test switches to continue to run a test.



Remote Test Box w/LED Indicators

RTB-02

Helps maintain a safe distance between the operator and test instrument when starting and restarting a test. Compatible with all models except SC6540.



E-Stop ESTOP

Immediately stop the flow of electric current to your instrument when the E-Stop is triggered. The E-Stop provides the safest and fastest way for a rescuer to save an operator from injury.



Test Verification Box TVB-2

The TVB-2 is a go/no-go daily test verification box designed to ensure that the failure detectors of an Associated Research electrical safety testing instrument are functioning properly. We designed the TVB-2 to verify Hipot, Insulation Resistance, Ground Bond, and Ground Continuity test functionality. If you perform daily verifications on your testing equipment, then the TVB-2 is an ideal solution. An accessory cord is available to customers who prefer to verify their test instrument using an adapter box.



TVB-2 Accessory Cord 39514

Accessory line cord for the TVB-2 allows convenient connection to a standard adapter box.



Leakage Current Verification Box LVB-2

Verify the failure detectors of your Associated Research Leakage Current Test instrument are functioning properly with this go/no-go load box.



Signal Tower Light 24V 40417

Our Signal tower light gives operators a visual indication of the status of the testing area. A green light indicates the Hipot tester is not outputting high voltage and the test area is safe. A red light indicates that the Hipot tester is active and to stay clear of the test area. Compatible with OMNIA® II Series, HypotULTRA® Series, Hypot® Series, HYAMP® Series, HypotMAX® Series, and LINECHECK II (620L).



Magnetic Hipot Return Cable CBLSR-05M

Magnetic Ground Bond Return Cable CBLHR-05M



2 Wire 40A Ground Bond Probe 38539

4 Wire 40A Ground Bond Probe 38538



High Voltage Pistol Probe with Switch

O.

High Voltage Probe 38081

Return Probe





Record, track and store your data with our brand new software as a service.

Compatible with Associated Research Hypot® Series, HypotULTRA® Series, OMNIA® II Series, HYAMP® Series, HypotMAX® Series, LINECHEK® II and SC6540. Also, SCI 290 Series, 260 Serie, and 440 Series.




- Unlimited Users
- Remote Instrument Connection
- Barcode Connection

- Intuitive User Interface
- Cloud / Local Storage
- Auto-File Loading



The platform's interface introduces an intuitive user experience making it easy to setup, run tests and view your reports.



Cloud storage ensures that your tests and data will never be lost or altered – all information is stored immediately to the cloud for access at any time.

Try it out for yourself with a free 30-day trial withstand.ikonixusa.com/auth/signup/create



OUR CONSULTING PACKAGES

Digital Packages

A web-based learning program. Choose from 2 packages; our Consulting on Demand or Customized Digital Package.

On-site Training Package

1-4 day on-site, handson training for your production line or R&D lab.

On-site Validation Package

2 or 4 day on-site training to completely satisfy your organization's validation needs.

 ${}^{\star}\mathsf{APAC}\ \mathsf{Region}\ \mathsf{Availability:}\ \mathsf{Digital}\ \mathsf{Packages}\ \mathsf{and}\ \mathsf{1-Day}\ \mathsf{On\text{-}site}\ \mathsf{Training}\ \mathsf{Program}.$

Visit **ikonixusa.com/consulting** to learn how we can help your team
WE WILL HELP MAKE SURE YOUR SYSTEM IS SAFE AND EFFECTIVE

COMMON SAFETY STANDARD REFERENCE CHART

Standard/	Testing	Dielectric	Withstand		Ground Bond/Continuity				
Harmonized Standard	Туре	Test Voltage	Max I.	Test Time	Test Current	V Limit	Max. R	Test Time	
IEC/UL 60601-1 3rd Edition	Performance	500 – 4000 VAC or 707 – 5656 VDC	No Breakdown	60 s	10-25 A	≤ 6 V	≤ 0.1 Ω	5 s	
Medical Electrical Equipment	Production*	1000 – 3000 VAC		1 or 60 s	10-25 A	≤ 6 V	≤ 0.1 Ω	5 s	
IEC 61730-2 UL 1703	Performance	1000 VAC + 2 x rated V or 2000 VAC + 4 x rated V	50 uA	60 s	2.5 x Max Over Current Protection	≤ 12 V	≤ 0.1 Ω	120 s	
Photovoltaic Modules & Panels	Production	1000 VAC + 2 x rated V or (1000 VDC + 2 x rated V) X 120%	50 uA	1 or 60 s		Conti	nuity		
IEC 60335-1 Household	Performance	500 – 2400 VAC x rated V + 2400 VAC	No Breakdown	60 s	≥ 10 A	≤ 12 V	0.1 – 0.2 Ω	≤ 120 s	
Electrical Appliances	Production	400 – 2500 VAC	5-30 mA	1 s	≥ 10 A	≤ 12 V	0.1 – 0.2 Ω	No time specified	
UL 60335-1 Household	Performance	500V – 2400 VAC x rated V + 2400 VAC	No Breakdown	60 s	40 A	≤ 6.5 V	≤ 0.5 Ω	120 s	
Electrical Appliances	Production	400 – 2500 VAC	5-30 mA	1 s	40 A	≤ 12 V	0.1 – 0.2 Ω	No time specified	
IEC 60598-1	Performance	500 – 4 x rated V + 2000 VAC	No Breakdown	60 s	≥ 10 A	≤ 12 V	≤ 0.5 Ω	60 s	
Luminaires	Production		Not	t Specified – Resp	onsibility of Manufact	urer			
UL 1598 Luminaires	Performance	1000 VAC – 1000 VAC x 2 x rated V	No Breakdown	60 s	30 A	≤ 4 V	≤ 0.1 Ω	120 s	
	Production	1200 VAC		1 s	Continuity $\leq 0.1 \Omega$ Continuity				
IEC/UL 61010-1 & CSA 22.2 No.	Performance	840 – 11940 VAC or 1200 – 7500 VDC	No Breakdown	5 – 60 s	25 or 30 A	≤ 10 V or ≤ 12 V	\leq 0.1 Ω or $<$ 4 V 0.133 Ω	60 or 120 s	
61010-1 Laboratory Control Test & Measurement Equipment	Production			5 s max ramp up 2 s dwell	Continuity				
EN 60204-1 Electrical	Performance	2 x rated V or 1000 VAC	No Breakdown	1 s	0.2 – 10 A	≤ 24 V	Refer to Section 18.2.2	No time specified	
Equipment of Machines	Production	Not Specified – Responsibility of Manufacturer							
UL 2202 Electric Vehicle Charging	Performance	500 VAC or 1000 VAC + 2 x rated V	No Breakdown	60 s	≤ 60 A	≤ 12 V	Continuity	120 – 240 s	
System Equipment	Production	1000 – 1700 VAC + 3.4 x rated V		60 or 1 s	Continuity				
IEC 61851-1 Electric Vehicle Conductive	Performance	1200 VAC + rated V or DC Equivalent	No Breakdown	60 s		Conti	nuity		
Charging System	Production		Not	t Specified – Resp	onsibility of Manufact	urer			
IEC 62368-1 Audi/Video,	Performance	1000 – 3000 VAC or 1414 – 4242 VDC	No Breakdown	60 s	≤ 40 A	≤ 12 V	≤ 0.1 Ω	60 s	
Information & Communication Technology Equipment	Production			1 – 6 s		Conti	nuity		

^{*}As a result of performing risk analysis, many medical device manufacturers are performing leakage tests as part of 100% production line testing.

Standard/	Testing	Suggested Model	nce	ulation Resistar	Ins	je	Earth Leakag		
Harmonized Standard	Туре	AR Instrument	Min. R	V Limit	Test Time	Max I.	Test Voltage		
IEC/UL 60601-1 3rd Edition	Performance	N/A 8206, 8207, 8256, 8257 or MedTEST		5-10 mA	110% x rated V				
Medical Electrical Equipment	Production*	7804 or 7854	N/A			5-10 mA	110% x rated V		
IEC 61730-2 UL 1703	Performance	3240, 8206, 8207, 8256, 8257 or MedTEST	40-400 MΩ	500 VDC or Max rated V	10 uA – 1 mA	10 uA – 1 mA	Max rated V		
Photovoltaic Modules & Panels	Production	3240, 3870 or 7850		N/A			N/A		
IEC 60335-1 Household	Performance	8256 or 8257		N/A		0.25 – 5.0 uA	1.06 x rated V		
Electrical Appliances	Production	7804		N/A			N/A		
UL 60335-1 Household	Performance	8256 or 8257		N/A		0.25 – 5.0 uA	1.06 x rated V		
Electrical Appliances	Production	7804		N/A			N/A		
IEC 60598-1 Luminaires	Performance	8206, 8207, 8256 or 8257	1-4 ΜΩ	500 VDC	60 s	0.5 – 10 mA	Rated V		
Lummanes	Production	Hypot® or 7850		acturer	onsibility of Manuf	ot Specified – Respo	No		
UL 1598 Luminaires	Performance	7804 or 7854	≥ 2 MΩ	500 VDC	No time specified		N/A		
	Production	Hypot® or 7850		N/A		N/A			
IEC/UL 61010-1 & CSA 22.2 No.	Performance	8256, 8257 or MedTEST		N/A		0.5 mA	< 300 V		
61010-1 Laboratory Control Test & Measurement Equipment	Production	3865 or 7850		N/A			N/A		
EN 60204-1 Electrical Equipment	Performance	7804 or 7854	≥ 1 MΩ	500 V	No time specified		N/A		
of Machines	Production	Hypot® or 7850		acturer	onsibility of Manuf	ot Specified – Respo	No		
UL 2202 Electric Vehicle Charging	Performance	8206, 8207, 8256, 8257 or MedTEST		N/A		0.5 – 0.75 mA or 5 mA	Rated V		
System Equipment	Production	Hypot® or 7850		N/A			N/A		
IEC 61851-1 Electric Vehicle Conductive	Performance	8206, 8207, 8256, 8257 or MedTEST	≥ 1 MΩ or ≥ 7 MΩ	500 V	60 s	Touch Current Only			
Charging System	Production	Hypot® or 7850		onsibility of Manufacturer			Not Specified – Respo		
IEC 62368-1 Audi/Video,	Performance	8206, 8207, 8256, 8257 or MedTEST	≥ 2 MΩ	500 V	60 s	0.25 – 3.5 mA	< 300 V		
Information & Communication Technology Equipment	Production	Hypot® or 7850		N/A			N/A		







HEADQUARTERS

28105 N. Keith Drive Lake Forest, IL 60045 USA **Telephone** +1-847-367-4077 Fax +1-847-367-4080 Email info@ikonixusa.com www.ikonixusa.com

Ikonix Taiwan

16F-2., No.237, Sec. 1, Datong Rd., Xizhi Dist., New Taipei City 221, Taiwan Telephone +886-2-21653066 Fax +886-2-21653077 Email contact@ikonixasia.com www.ikonixasia.com

Ikonix Asia

Unit D3-5-2 (2ND Floor) Block D3, Dana 1 Commercial Centre, Jalan PJU 1A/46, 47301 Petaling Jaya, Selangor, Malaysia **Telephone** +60-3-78429168 Fax +60-3-78426168 Email contact@ikonixasia.com www.ikonixasia.com







We Have Local Sales Offices Throughout the World

To find your nearest representative visit us at ikonixasia.com