

Instruments for Electrical Safety Compliance Testing



Experts In Electrical Safety Compliance.®

Hipot • Ground Bond • Insulation Resistance • Leakage Current • Functional Run Medical Test Systems • HV/HC Multiplexers • Software Solutions

CUSTOMER HAPPINESS PROMISE


We aim to provide an amazing experience and quality testers that last a long time. If you're not satisfied with your tester, return it within 45 days for a full refund. Calibrate annually with us, or one of our authorized partners, and we'll extend your warranty an additional year for the service life of your tester, and at least five years after discontinuation. If it breaks during that time, we promise to fix it for free (unless abuse or excessive damage is present). When your tester reaches the end of its service life, we'll responsibly recycle it and give you a discount on a replacement.



*Annual calibration and inspection must be made in each successive year starting one year after the original purchase date in order to remain eligible for extended warranty coverage beyond the standard warranty period (five years).

5 YEAR WARRANTY

Your new tester is warranted to be free from defects in workmanship and material for a period of (5) years from date of shipment.





ONGOING SUPPORT

We work to provide the best service and support in the industry. With decades of industry experience we are the pros you can trust to help you be compliant to NRTL standards. We'll work closely with you to help you achieve your goals. We've built a worldwide network of knowledgable partners, so you're covered no matter where you are.



A HISTORY OF INNOVATION

 We introduced the first battery operated Megohmmeter, the Vibrotest, in the United States. We commenced the first Cable Testing/Fault Location school known as ARU. ARU continued for over 25 years. We introduced the first complete family of microprocessor-controlled electrical safety instruments. We developed the first mobile app in the electrical safety testing industry. We launched the first mobile app in the electrical safety testing industry. We launched the Applications Consulting program. We launched the Applications Consulting program. We launched Withstand®, a Software as a Service (SaaS) 	1936	Associated Research was founded.	2001	We released our patented safety feature, SmartGFI®, to provide our customers with
We commenced the first Cable Testing/Fault Location school known as ARU. ARU continued for over 25 years. We introduced the first complete family of microprocessor-controlled electrical safety instruments. We developed the first mobile app in the electrical safety testing industry. We launched the first mobile app in the electrical safety testing industry. We launched the Applications Consulting program. We launched the first mobile app in the electrical safety testing industry. We launched the Applications Consulting program. We launched the first mobile app in the electrical safety testing industry. We launched the first mobile app in the electrical safety testing industry. We launched the first mobile app in the electrical safety testing industry. We launched the first mobile app in the electrical safety testing industry. We launched the first mobile app in the electrical safety testing industry. We launched the first mobile app in the electrical safety testing industry. We launched the first mobile app in the electrical safety testing industry. We launched the first mobile app in the electrical safety testing industry. We launched the first enterties app in the electrical safety testing industry. We launched the first enterties app in the electrical safety testing industry. We launched the first enterties app in the electrical safety testing industry. We launched the first enterties app in the electrical safety testing industry. We launched the first enterties app in the electrical safety testing industry. We launched the Applications Consulting program. Associated Research joins the IKONIX family to become and IKONIX Brand.	1939	first battery operated Megohmmeter, the Vibrotest,		maximum operator protection during high voltage testing.
1993 We introduced the first complete family of microprocessor-controlled electrical safety instruments. 1995 We developed the first mobile app in the electrical safety testing industry. 2017 We launched the Applications Consulting program. We launched the Applications Consulting program. We Introduced Withstand®, a Software as a Service (SaaS) platform, that is a cloud storage of your tests and data in one platform. We introduced Autoware, the first software package for automated instrument control,	1966	We commenced the first Cable Testing/Fault Location school known as ARU. ARU	2012	safety compliance analyzer with a built-in AC power
1995 We developed the first multi-function electrical safety compliance analyzer. 2017 Consulting program. We launched the Applications Consulting program. We Introduced Withstand®, a Software as a Service (SaaS) platform, that is a cloud storage of your tests and data in one platform. Platform. We Introduced Withstand®, a Software as a Service (SaaS) platform, that is a cloud storage of your tests and data in one platform. We introduced Autoware, the first software package for automated instrument control,	1993	We introduced the first complete family of microprocessor-controlled electrical safety	2013	app in the electrical safety
We Introduced Withstand®, a Software as a Service (SaaS) platform, that is a cloud storage of your tests and data in one platform. We introduced Autoware, the first software package for automated instrument control, We Introduced Withstand®, a Software as a Service (SaaS) platform, that is a cloud storage of your tests and data in one platform. Associated Research joins the IKONIX family to become and IKONIX Brand.	1995	We developed the first multi-function electrical	2017	• • •
We introduced Autoware, the first software package for automated instrument control, the IKONIX family to become and IKONIX Brand.	1997	We released the first electrical safety instrument with a built-in multiplexer for	2020	a Software as a Service (SaaS) platform, that is a cloud storage of your tests and data in one
	1999	the first software package for automated instrument control,	2021	the IKONIX family to

FOCUSED ON EDUCATION

With over 80 years of industry experience, we have the resources and expertise to assist you with your educational needs throughout the life of your product.

- Quick Start Videos
- On-Site Training
- Quick Start Guides White Papers & Articles

SERVING THE COMMUNITY

portfolio.

2023

Ikonix globalizes it's product




We donate a portion of our profits to raising awareness about the dangers of electricity.

PRODUCT REFERENCE CHART

	\sim		40A		/WW	\	F	\sim	
	AC Hipot	DC Hipot	Ground Bond	Ground Continuity	Insulation Resistance	Leakage Current	Functional Run	Built-in AC Power	
Hypot®									
3805	•			•					
3855	•			•	•				
3865	•	•		•					
3870	•	•		•	•				
HypotULTRA®									
7800	500 VA	•		•	•				
7804	•	•	•	•	•				
7820	•			•					
7850	•	•		•	•				
7854	500 VA	•	•	•	•				
OMNIA® II									
8204	•	•	•	•	•				
8254	500 VA	•	•	•	•				
8206	•	•	•	•	•	•	•		
8256	500 VA	•	•	•	•	•	•		
8207	•	•	•	•	•	•	•	•	
8257	500 VA	•	•	•	•	•	•	•	
HYAMP®									
3240			•						
HypotMAX [®]									
7705	•								
7710		•							
7715	•								
7720		•							
LINECHEK® II									
620L SC6540						•	•		
5C6540 HN									
HH									
HG									
GN									
GIN									

GG

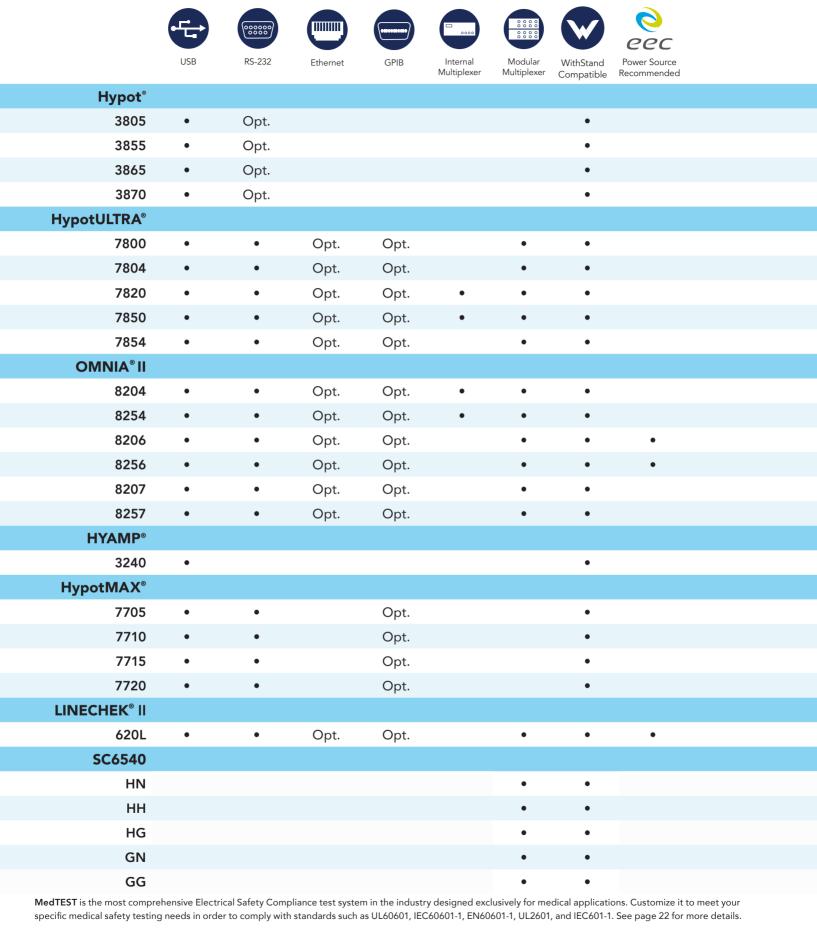



Our Hypot® Series raises the bar for production line Hipot testing. Improve traceability with onboard data storage and easily transfer test result data and test settings via convenient front panel USB. Take the guesswork out of your production line with the direct barcode connection to quickly associate products with pre-programmed test files. We've included advanced features like improved security and a touch screen interface that provides custom pop-up prompts displayed before each test step. We've dramatically reduced the weight and footprint of the Hypot® Series to make safety compliance a less strenuous ordeal. Quickly interconnect with the HYAMP® Series to form a complete safety compliance system.



Find the Model that Fits Your Testing Needs



SAFETY & PRODUCTIVITY FEATURES







SmartGFI[©] Automatic operator shock protection

Interlock Easily disable HV output

Data Transfer Easily import/ export test files and data via USB







Multiple Barcode Capability Languages Direct barcode Multiconnection Language user interface

PLC Remote Basic PLC relay control







Prompt & Hold Provides alerts & instructions

protection

Advanced User Security Interconnect with & password a complete test system







Ramp-HI® Reduce ramp DC Hipot

Confirms proper DUT connection

FailCHEKTM Confirms detection



available

Accredited WithStand® Automation Accredited calibration



Storage Save up to 1,500 Test Results onboard

INPUT SPECIFICATIONS					
Voltage	100 – 120 VAC	/ 200 – 2	40 VAC ± 10%	Auto Range	
Frequency	50/60 Hz ± 5%				
Fuse	3.15 A, Fast Blo	ow 250 VA	AC		
DIELECTRIC WIT	HSTAND TES	г морі	≣		
Output Rating	3805/3855/ 3865/3870		20 mAAC 7.5 mADC (386	55/3870 only)	
Maximum Limit	3805/3855/ 3865/3870	AC	Range: Resolution:	0.00 – 20.00 mA 0.01 mA	
		DC	Range: Resolution: Accuracy:	$0-7500~\mu A$ $1~\mu A$ AC and DC \pm (2% of setting + 2 counts)	
Minimum Limit	3805/3855/ 3865/3870	AC	Range: Resolution:	0.000 – 9.999 mA 0.001 mA	
		DC	Range: Resolution: Accuracy:	0.0 – 999.9 μ A 0.1μ A AC and DC \pm (2% of setting + 2 counts)	
Arc Detection	Range:	1 – 9 (9	is most sensit	ive)	
Ground Fault Interrupt	GFI Trip Currer	nt: 450 μ <i>Α</i>	A max (AC or D	OC), Fixed	
apt	HV Shut Down	Speed: <	1 msec		
Current Display	3805/3855/ 3865/3870	AC	Range 1: Range 2:	0.000 – 4.000 mA 3.50 – 20.00 mA	
		DC	Range 1: Range 2: Range 3:	0.0 μA – 400.0 μA 0.350 mA – 4.000 mA 3.50 mA – 7.50 mA	
			Accuracy:	All Ranges ± (2% of reading + 2 counts)	
DC Output Ripple	≤ 5% Ripple rm	ıs at 6 kV	DC @ 7.5 mA F	Resistive Load	
RAMP-HI Selectable	Range: 0.0 – 7,5	500 μΑ, ι	Jser Selectable	e	
Charge-LO	0 – 350 μA DC	or Auto S	Set		
Discharge Time	< 50 msec for no load, < 100 msec for capacitive load The maximum capacitive load vs. output voltage: $1\mu F < 1KV \qquad 0.08\mu F < 4KV \\ 0.75\mu F < 2KV \qquad 0.04\mu F < 5KV \\ 0.5\mu F < 3KV \qquad 0.015\mu F < 6KV$				
AC Voltage Waveform/	Sine Wave, Cre	st Factor	= 1.3 – 1.5		
Frequency	Range:	50 or 60) Hz, User Sele	ectable	
Dwell Timer	Range:		.2-999.9 sec (0 .4-999.9 sec (0		
Ramp Timer	Range:		Jp: 0.1 – 999.9 Down: AC 0.0 - DC 0, 1.		
Ground Continui- ty Current	DC 0.1A ± 0.01	A, fixed			
Ground Conti- nuity Maximum Limit Minimum Limit	Range: Resolution: Accuracy:	n: 0.01 Ω			
Ground Conti- nuity Auto Offset	Range: Resolution: Accuracy:	0.00 – 0 0.01 Ω ± (3% o	0.50Ω f setting + 0.0	2 Ω)	

INSULATION RESIST.	ANCE TEST MOI	DE		
Voltage Setting	Range: Resolution: Accuracy:	30 – 1,000 VDC 1 V ± (1.5% of setting + 5 V)		
Resistance Display	Range:	1 – 50,000 ΜΩ		
	$\begin{tabular}{ll} Resolution: & 30 - 99 V \\ MΩ & MΩ \\ 0.001 & 1.000 - 1. \\ 0.01 & 2.00 - 19. \\ 0.1 & 20.0 - 19. \\ 1 & 200 - 10. \\ \end{tabular}$	MΩ $MΩ$ $MΩ999 1.000 – 1.999 1.000 – 9.99999 2.00 – 19.99 10.00 – 99.999.9 20.0 – 199.9 100.0 – 999.9$		
	Accuracy:	\pm (8% of reading+2 counts) at test voltage 30 – 499 V and 1.00–999.9 $M\Omega$		
	± (5% of reading	$500-1000$ V $_{19}$ + 2 counts) for 1.00 – 999.9 M $_{\Omega}$ $_{19}$ + 2 counts) for 1000 – 9999 M $_{\Omega}$ $_{10}$ $_{10}$ + 2 counts) for 10000 – 50,000 M $_{\Omega}$		
HI & LO-Limit	Range: Resolution:	0, 1.00 – 99.99 M Ω (0=OFF, HI-Limit ONLY) 0.01 M Ω 1000-50000 1 M Ω		
	Range: Resolution:	100.0 – 999.9 MΩ 0.1 MΩ		
	Accuracy:	At test voltage 500-1000 V \pm (2% of setting + 2 counts) for 1.00 – 999.9 M Ω \pm (5% of setting + 2 counts) for 1000 – 9999 M Ω \pm (15% of setting + 2 counts) for 10000 – 50,000 M Ω		
Charge-LO	Range: 0.000 – 3.500 μA DC or Auto Set			
Ramp Timer	Range:	Ramp-Up: 0.1 – 999.9 sec Ramp-Down: 0, 1.0 – 999.9 sec, (0=OFF)		
Delay Timer	Range:	0.5 – 999.9 sec (0=OFF)		
Dwell Timer	Range:	0, 0.5 – 999.9 sec (0=continuous)		
GENERAL SPECIFICA	TIONS			
Remote Control and Signal I/O		t, Hardware Interlock, File Recall il, Test-in-Process, Reset-Out, Start-Out		
Vmax	Displays the maxir a breakdown	num voltage value recorded during		
lmax	Displays the maxir	num leakage current value read during a test		
Memories	50 steps 1500 test results			
Interface	USB standard			
Language		al Chinese, Simplified Chinese, Turkish, ish, German, French		
Security	Multiple user setu	ps with ID and password		
Dimensions (W x H x D)	3805/3855/ 3865/3870	8.5" x 3.5" x 11.9" (215 mm x 88.1 mm x 300 mm)		
Weight	3805/3855/ 3865/3870	12 lbs (5.46 kgs)		

For reading specifications, please refer to the user manual.

Why We Use Counts

Associated Research publishes some specifications using "counts" which allows us to provide a better indication of the instrument's capabilities across measurement ranges. A count refers to the lowest resolution of the display for a given measurement range. For example, if the resolution for voltage is 1V then 2 counts = 2 V.

Specifications subject to change without notice.

HypotULTRA®

The Most Flexible and Feature-Rich Automated Dielectric Analyzer Available



Our HypotULTRA® models provide all the tools you need to modernize your production line with best-in-class 4-in-1 test capability and a slim 2U design. We've added 40A AC Ground Bond test capability to HypotULTRA's already impressive feature list for manufacturers that aim to adopt best testing practices without sacrificing productivity. Whether you're looking to improve traceability with onboard data storage, increase efficiency with our intuitive touch screen interface and direct barcode scanner connection, or automate with a variety of communication interfaces, HypotULTRA was designed to take your production line to the next level.



Find the Model that Fits Your Testing Needs



^{*}Meets 200 mA short circuit requirements

AVAILABLE INTERFACES









USB

Ethernet (Optional)

GPIB (Optional

SAFETY & PRODUCTIVITY FEATURES







SmartGFI® Automatic operator shock protection

Remote Safet Interlock Easily disable HV output

Data Transfer Easily import/ export test files and data via USB



Barcode Capability Direct barcode connection



Multiple Languages Multi-Language user



lle Ground Bond ges Voltage Drop - Monitor e user voltage drop vs resistance







Internal Multiplexer Available with optional HV multiplexer (4 or 8 ports)



Modular Multiplexer Compatible with SC6540 multiplexers





detection



Prompt & Hold Provides alerts & instructions

between tests



WithStand® Automation Software







Ramp-HI® Reduce ramp time during DC Hipot



Confirms

proper DUT



PLC Remote Basic PLC relay control



Negative DC Hipot Reverse polarity DC Hipot (optional)



On Board Data Storage Save up to 100,000 Test Results onboard

HypotULTRA® Series

						HypotULTRA® Series
INPUT SPECIFICA	ATIONS			INSULATION RESISTA	ANCE MODE	(Models 7800/7804/7850 & 7854 Only)
Voltage	100 – 120 VA	AC / 200 – 240	VAC ± 10% Auto Range	Charging Current HI	Maximum > 2	0 mA peak
Frequency	50/60 Hz ± 5%		and LO-Limit	Range:	0.10 MΩ – 99.9 MΩ (HI-Limit: 0=OFF)	
Fuse	780	4/7820/7850:	6.3A, Slow Blow 250 VAC		Resolution: Accuracy:	0.01 M Ω ± (2% of setting + 2 counts)
AC WITHSTAND	TEST MODE	7800/7854:	15A, Fast Blow 250 VAC		Range: Resolution:	100.0 MΩ – 999.9 MΩ 0.1 MΩ
			•		Accuracy:	1,000 – 9,999 ± (5% of setting + 2 counts)
Output Voltage	Range: Resolution: Accuracy:	0 – 5,000 VA 1 VAC ± (1.5% of se			Range: Resolution:	1,000 MΩ – 50,000 MΩ 1 MΩ
Output Frequency	50/60 Hz ± 0).1%, User Sele	ection		Accuracy:	10,000 – 50,000 ± (15% of setting + 2 counts)
Output Waveform	Sine Wave, C	Crest Factor =	1.3 – 1.5	Ramp Up Timer	Range:	0.1 – 999.9 sec
Output Regu-	± (1% of out	put + 5V)		Ramp Down Timer	Range:	1.0 – 999.9 sec
ation				Dwell Timer	Range:	0.5 – 999.9 sec (0=Continuous)
HI and LO-Limit Total	Total	Range: Resolution:	0.000 – 9.999 mA 0.001 mA	Delay Timer	Range:	0.5 – 999.9 sec
		Range:	10.00 – 40.00 mA (10 – 99.99 mA, Models 7800/7854)	Charge-LO		μA or Auto Set
		Resolution: Accuracy:	0.01 mA ± (2% of setting + 2 counts)	CONTINUITY TEST M	ODE (All Mo	dels)
	Real	Range:	7804/7820/7850 ± (2% of setting + 6 counts) 7800/7854 0.000 – 9.999 mA	Output Current, DC	0.01 A for 10.0	– 1.000 Ω, 0.1 A for 1.01 – 10.00 Ω 01 – 100 Ω, 0.001 A for 101 – 1,000 Ω 001 – 10,000 Ω, 1 A is Max
	Real	Resolution: Range:	0.001 mA 10.00 – 40.00 mA (10 – 99.99 mA	Resistance Display Max	Range:	0.000 – 1.000 Ω
		Resolution: Accuracy:	7800/7854) 0.01 mA ± (3% of setting + 50 μA)	& Min Lmt	Resolution: Accuracy:	0.001 Ω ± (1% of setting + 3 counts)
Ramp Up Timer Ramp Down Timer Dwell Timer	Range: Range:	0.1 – 999.9 se 0.0 – 999.9 se	ec		Range: Resolution: Accuracy:	$1.01 - 10.00 \Omega$ 0.01Ω $\pm (1\% \text{ of setting} + 3 \text{ counts})$
Ground Conti- nuity		Range: 0, 0.2 – 999.9 sec (0=Continuous) Current: DC 0.1A ± 0.01A, fixed			Range: Resolution: Accuracy:	$10.1 - 100.0 \Omega$ 0.1Ω $\pm (1\% \text{ of setting } + 3 \text{ counts})$
Current	Max. Ground	Max. Ground Resistance: 1.0 Ω ± 0.1 Ω			Range:	101 – 1,000 Ω
Arc Detection	Range:	•			Resolution: Accuracy:	1 Ω ± (1% of setting + 3 counts)
Output Voltage	Range:	0 – 6000 VD0	800/7804/7850 & 7854 Only)		Range: Resolution:	1,001 – 10,000 Ω 1 Ω
	Resolution: Accuracy:	1 V ± (1.5% of se	tting + 5 V)	Dwell Timer	Accuracy:	± (1% of setting + 10 counts) 0, 0.4 – 999.9 sec (0=Continuous)
DC Output Ripple	<4% (6 KV/1	0 mA at Resist	ive Load)	Resistance Offset	Range:	0.000 – 10.00 Ω
HI and LO-Limit	Range: Resolution:	0.0000 – 0.99 0.0001 μA	999 μΑ		Range:	dels 7804 & 7854 Only)
	Accuracy:		ing + 10 counts), Low Range is ON		· ·	3.00 – 8.00 VAC
	Range: Resolution: Accuracy:	1.000 – 9.999 0.001 µA ± (2% of sett	P μA ing + 10 counts), Low Range is ON	Output Voltage (Open Circuit Voltage)	Range: Resolution: Accuracy:	0.01 VAC ± (2% of setting + 3 counts) Open Circuit
	Range: Resolution: Accuracy:	10.00 – 99.99 0.01 µA ± (2% of sett	P μA ing + 10 counts), Low Range is ON	Output Current	Resolution:	1.00 – 40.00 A 0.01 A ± (2% of setting + 2 counts)
	Range: Resolution: Accuracy:	100.0 – 999.9 0.1 μΑ ± (2% of sett	P μA ing + 2 counts)	Maximum Loading	1.00 - 10.00 A, $0 - 600$ mΩ $10.01 - 30.00$ A, $0 - 200$ mΩ $10.01 - 40.00$ A, $0 - 150$ mΩ	
	Range: Resolution: Accuracy:	1,000 – 10,00 1 µA	00 μA range (7804/54) 00μA range (7800/50) ing + 2 counts)	HI and LO-Limit	Range:	0 – 150 mΩ for 30.01 – 40.00 A 0 – 200 mΩ for 10.01 – 30.00 A 0 – 600 mΩ for 1.00 – 10.00 A
Ramp Up Timer	Range:	0.4 - 999.9 se	ec, Low Range is OFF ec, Low Range is ON		Resolution: Accuracy:	1 mΩ ± (2% of setting + 2 counts)
Ramp Down Timer	Range:		9.9 sec (0=OFF)		Range: Resolution: Accuracy:	0 – 600 mΩ 1 mΩ ± (3% of setting + 3 counts)
Dwell Timer	Range:		P sec (0=Continuous) P sec, Low Range is ON	Dwell Timer	Range:	0, 0.5 – 999.9 sec (0=Continuous)
Ramp-HI Select- able	Range:	0 – 20 mA se	lectable	Milliohm Offset	0 – 200 mΩ	., . ,
Charge-LO	Range:	0.0 – 350.0 μ	A DC or Auto Set	Voltage Offset	0.0 - 6.0 V	
Discharge Time			ms for capacitive load	GENERAL SPECIFICA	TIONS	
Maximum Capacitive Load DC Mode	1μF < 1kV 0.75 μF < 2 k 0.5 μF < 3 k\	0.0 uF <		Memory	2,000 steps, 2 100,000 test r	00 steps per test file max esults
Arc Detection		1 – 9 (9 is mo		Mechanical	Bench or rack	mount (2U height) with feet
			els 7800/7804/7850 & 7854 Only)	Interface	Standard: USE Optional: GPI	3, RS-232 B (IEEE-488.2), Ethernet
Output Voltage,	Range:	10 – 1,000 VI	OC .	SmartGFI®	0, 0.4 – 5.0 mA	A (0=OFF)
DC '	Resolution: Accuracy:	1 VDC ± (1.5% of se	tting + 2 counts)	Dimensions (W x H x D)	16.92" x 3.50"	x 15.75" (430 x 88.1 x 400mm)
	Range: Resolution:	1,001 – 6,000 1 VDC ± (1.5% of se) VDC	Weight	7800: 7804: 7820:	45 lbs (20.4 kg) 46.3 lbs (21 kg) 35 lbs (15.9 kg)

For reading specifications, please refer to the user manual. Specifications subject to change without notice.

The Most Advanced Electrical Safety Compliance Analyzer in the Industry



Our OMNIA® II Series is a complete line of multi-function electrical safety compliance analyzers designed to satisfy even the most demanding application requirements. We've included exclusive productivityenhancing features and the latest in safety technology to make this product line the envy of the industry. With 6 models to choose from, a multi-language menu system and a variety of automation interfaces available, the OMNIA® II is ready for global deployment.



Find the Model that Fits Your Testing Needs



*Meets 200 mA short circuit requirements

AVAILABLE INTERFACES









RS-232 Ethernet

GPIB

SAFETY & PRODUCTIVITY **FEATURES**







Automatic operator shock protection

Easily disable HV output

Hold Provides alerts between tests



Language user

interface

Multiple Languages Multi-



Active Link® Continuous power during



Customize you own shortcut test steps



DualCHEK[©] Simultaneous Hipot and



Multiplexer Available with optional HV multiplexer (8 ports)



Multiplexer Compatible with SC6540 multiplexers







FailCHEK™ Confirms failure detection



Cal-Alert® Tracks and alerts for calibration



Charge-LO® Reduce ramp Confirms



Arc Detection

High proper DUT connection frequency filter for corona detection



time during DC Hipot

WithStand® Automation



Accredited Cal Accredited calibration options

available



Voltage Drop Monitor voltage drop vs resistance

INPUT SPECIFICA	ATIONS		
Voltage	115/230 V Auto	Range, ± 15 S	% Variation
Frequency	50/60 Hz ± 5%		
Fuse	115 VAC, 230 V	AC – 10 A Slo	w Blow 250 VAC
DIELECTRIC WIT	HSTAND TES	T MODE	
Output Rating	5 kV @ 50 mAA 5 kV @ 100 mA 6 kV @ 20 mAD	AC (Models 82	25X)
Voltage Setting	Resolution: Accuracy:	1 V ± (1.5% of se	tting + 5 volts)
HI and LO-Limit	AC Total	Range: Resolution:	0.000 – 9.999 mA 0.001 mA
		Range:	10.00 – 50.00 mA (100.00 mA, models 825X) 0.01 mA
		Accuracy:	± (2% of setting + 2 counts)
	AC Real	Range: Resolution:	0.000 – 9.999 mA 0.001 mA
		Range:	10.00 – 50.00 mA (100.00 mA, models 825X) 0.01 mA
		Accuracy:	± (3% of setting + 50 μA)
	DC	Range: Resolution:	0 – 999.9 μA 0.1 μA
		Range: Resolution:	1,000 – 20,000 μA 1 μA
		Accuracy:	± (2% of setting + 2 counts)
Arc Detection	Range:	1 – 9 (9 is m	ost sensitive)
Ground Continuity	Current: DC 0. Max. Ground R		
Ground Fault Interrupt	GFI Trip Currer HV Shut Down		0 mA (AC or DC)
DC Output Ripple	≤ 4% Ripple rm	s at 5 kVDC at	20 mA Resistive Load
Discharge Time	≤ 50 ms No Loa	ad, < 100 ms f	or Capacitive Load
Max Capacitive Load, DC Mode	1 μF < 1 kV 0.75 μF < 2 kV 0.5 μF < 3 kV		18 μF < 4 kV 14 μF < 6 kV
AC Output Waveform	Sine Wave, Cre	st Factor = 1.3	3 – 1.5
Output Frequency	Range:	60 or 50 Hz,	User Selection (400/800 Hz optional)
Output Regulation	± (1% of output voltage rang		o load to full load and over input
Dwell Timer	Range: Range:		9 sec (0=Continuous) 9 sec (0=Continuous)
Ramp Timer	Ramp-up: AC 0.1 – 999.9 sec, DC 0.4 – 999.9 sec Ramp-Down: AC 0.0 – 999.9 sec, DC 0.0 , 1.0 – 999.9 sec (0=Continuous)		
INSULATION RES	SISTANCE TES	T MODE	

 $\begin{array}{c} \text{Range:} \quad 30-6000\,\text{VDC} \\ \\ \text{Range:} \quad 0.05\,\text{M}\Omega-99.99\,\text{M}\Omega \\ \text{Resolution:} \quad 0.01\,\text{M}\Omega \end{array}$

Range: $100.0 \text{ M}\Omega - 999.9 \text{ M}\Omega$ Resolution: $0.1 \text{ M}\Omega$

Range: $1,000 \text{ M}\Omega - 50,000 \text{ M}\Omega$ Resolution: $1 \text{ M}\Omega \text{ (HI-Limit: 0=OFF)}$

Ramp-up: 0.1 – 999.9 sec Ramp-Down: 0.0, 1.0 – 999.9 sec (0=Continuous)

Range: 0.5 – 999.9 sec (0=Continuous)

Voltage Setting

HI and LO-Limit

Ramp Timer

Delay Timer

	C
	0
	Re Di
	Н
)	
	D
	М
	R
	DI
optional)	
nput	
	D:
	D
c	Se

		OMINIA II Series
GROUND BOND	TEST MODE	
Output Voltage (Open Circuit Limit)	Range:	3.00 – 8.00 VAC
Output Frequency	Range:	60 or 50 Hz, User Selectable
Output Current	Range: Resolution: Accuracy:	1.00 – 40.00 A 0.01 A ± (2% of setting + 0.02 A)
Maximum Loading	1.00 – 10.00 A, 10.01 – 30.00 A 30.01 – 40.00 A	Λ , $0-200 \mathrm{m}\Omega$
HI and LO-Limit	Range: Resolution: Accuracy:	$\begin{array}{l} 0-150 \ m\Omega \ for \ 30.01-40.00 \ A \\ 0-200 \ m\Omega \ for \ 10.01-30.00 \ A \\ 0-600 \ m\Omega \ for \ 1.00-10.00 \ A \\ 1 \ m\Omega \\ \pm (2\% \ of \ reading + 2 \ m\Omega) \end{array}$
	Range: Resolution: Accuracy:	$0-600~m\Omega~for~1.00-5.99~A$ 1 m Ω ± (3% of reading + 3 m Ω)
Dwell Timer	Range:	0.5 – 999.9 sec (0=Continuous)
Milliohm Offset	Range:	$0-200~\text{m}\Omega$
CONTINUITY TE	ST MODE	
Output Current	DC 0.01 A ± 0.	00001 A
Resistance Display	Range:	0.00 – 10000 Ω
HI and LO-Limit	Range: Resolution:	1: $0.00 - 10.00 \Omega$ 0.01Ω
	Range 2: Resolution:	10.1 – 100.0 Ω 0.1 Ω
	Range 3: Resolution: Accuracy:	101 – 1,000 Ω 1 Ω ± (1% of reading + 3 counts)
	Range 4: Resolution: Accuracy:	1,001 – 10,000 Ω 1 Ω ± (1% of reading + 10 counts) (Max Limit: 0=OFF)
Dwell Timer	Range:	0.0, 0.3 – 999.9 sec (0=Continuous)
Milliohm Offset	Range:	0.00 – 10.00 Ω
RUN TEST MODE	(Models 82)	X6 & 82X7 only)
DUT Power	Voltage: Current: Range: Resolution: Accuracy:	0 – 277 VAC single phase unbalanced 16 AAC max continuous 0.0 – 277.0 VAC Full Scale 0.1 V ± (1.5% of reading +0.2 V), 30.0 – 277.0 VAC Short Circuit Protection: 23 AAC, Response Time < 3 sec
Delay Time Setting	Range:	0.2 – 999.9 seconds
Dwell Time Setting	Range:	0.1 – 999.9 seconds (0=Continuous)

OMNIA® I	l Series						
RUN TEST MC	DE CONTINUE	D (Models 82	2X6 & 82X7 only)				
Trip Point Settings	Voltage						
& Metering	Volt-Hi Volt-LO	Range: Resolution: Accuracy:	30.0 – 277.0 VAC 0.1 V ± (1.5% of setting + 0.2 V), 30.0–277 VAC				
	Current						
	Amp-HI Amp-LO	Range: Resolution: Accuracy:	0.0 – 16.00 AAC 0.01 A ± (2.0% of setting + 2 counts)				
	Watts						
	Power-HI Power-LO	Range: Resolution: Accuracy:	0 – 4,500 W 1 W ± (5.0% of setting + 3 counts)				
	Power Factor	Power Factor					
	PF-HI PF-LO	Range: Resolution: Accuracy:	0.000 – 1.000 0.001 ± (8% of setting + 2 counts)				
	Leakage Current						
	Leak-HI Leak-LO	Range: Resolution: Accuracy:	0.00 – 10.00 mA (0=OFF) 0.01 mA ± (2% of setting + 2 counts)				
Timer Display	Range: Resolution: Accuracy:	0.0 – 999.9 sec 0.1 second ± (0.1% of reac	conds ding + 0.05 seconds)				
LEAKAGE CUI	RRENT TEST MO	DDE (Models	82X6 & 82X7 only)				
DUT Power	Voltage: Current:	0 – 277 VAC 16 AAC max continuous					
	Voltage Display	Range: Resolution: Accuracy:	0.0 – 277.0 VAC Full Scale 0.1 V ± (1.5% of reading +0.2 V), 30.0 – 277.0 VAC				
	Short Circuit Protection:	23 AAC, Response Time < 3 s					
Reverse Power Switch	Reverse polarity ON: Reverse pov OFF: Normal AUTO: Automati	ver	elect ON/OFF/AUTO				
Neutral Switch	ON/OFF selection	n for single fau	lt condition				
Ground Switch	ON/OFF selection for Class I single fault condition						

Surface to Surface (PH – PL) Surface to Line (PH – L) Ground to Line (G – L)

Range: 0.0 μA ~ 999.9 μA 1000 μA ~ 10.00 mA Resolution: 0.1 μA / 1 μA / 0.01 mA

Probe Setting

Touch Current High Limit (rms)

LEAKAGE CURF	RENT TEST MO	DE CONTINUED (Models 82X6 & 82X7 only)			
Touch Current	Range 1:	$0.0~\mu A\sim 32.0~\mu A,$ frequency DC, 15 Hz – 1 MHz			
Display (rms)	Range 2:	$28.0~\mu A \sim 130.0~\mu A,$ frequency DC, 15 Hz – 1 MHz			
	Range 3:	120.0 μ A ~ 550.0 μ A, frequency DC, 15 Hz – 1 MHz			
	Resolution for Ranges 1, 2, 3:	0.1 μΑ			
	Accuracy for Ranges 1, 2, 3:	DC: 15 Hz < f <100 KHz: \pm (2% of reading + 3 counts) 100 KHz < f < 1 MHZ: \pm 5% of reading (10.0 μ A – 999.9 μ A)			
	Range 4:	$400 \mu A \sim 2100 \mu A$, frequency DC, 15 Hz – 1 MHz			
	Range 5:	800 μA ~ 8500 μA, frequency DC, 15 Hz – 1 MHz			
	Resolution for Ranges 4 & 5:	1 μΑ			
	Accuracy for Ranges 4 & 5:	DC: 15 Hz < f <100 KHz: \pm (2% of reading + 3 counts) 100 KHz < f < 1 MHZ: \pm 5% of reading (10 μ A $-$ 8500 μ A)			
	Range 6:	8.00 mA ~ 10.00 mA, frequency DC 15 Hz – 100 kHz			
	Resolution:	0.01 mA			
	Accuracy:	DC: 15 Hz < f < 100 KHz: ± 5% of reading (0.01 mA -10.00 mA)			
Touch Current	Range 1:	$0.0~\mu A\sim 32.0~\mu A$, frequency DC – 1 MHz			
Display (Peak)	Range 2:	28.0 μA ~ 130.0 μA, frequency DC – 1 MHz			
	Range 3:	120.0 μ A ~ 550.0 μ A, frequency DC – 1 MHz			
	Resolution for Ranges 1, 2, 3:	0.1 μΑ			
	Accuracy for Ranges 1, 2, 3:	DC: \pm (2% of reading + 2 μ A) 15 Hz < f < 1 MHZ: \pm 10% of reading + 2 μ A			
	Range 4:	400 μA ~ 2100 μA, frequency DC – 1 MHz			
	Range 5:	1800 A ~ 8500 μA, frequency DC – 1 MHz			
	Resolution for Ranges 4 & 5:	1 μΑ			
	Accuracy for Ranges 4 & 5:	DC: \pm (2% of reading + 2 μ A) 15 Hz < f < 1 MHz: \pm (10% of reading + 2 μ A)			
	Range 6:	8.0 mA ~10.00 mA, frequency DC – 100 KHz			
	Resolution:	0.01 mA			
	Accuracy:	DC: ± (2% of reading + 3 counts) 15 Hz < f < 100 KHz: ± (10% of reading + 2 counts)			
MD Circuit Module	MD1: UL544NP, UL484 , UL923, UL471, UL867, UL697 MD2: UL544P MD3: IEC 60601-1 MD4: UL1563 MD5: IEC60990 Fig4 U2, IEC62368-1, IEC60335-1, IEC60598-1, IEC60065, IEC61010 MD6: IEC60990 Fig5 U3, IEC60598-1 MD7: IEC62368-1, IEC61010-1 FigA.2 (2K ohm) for Run function MD8: IEC60990/IEC62368-1 Fig4 U1				
External MD	Basic measuring	element 1 kΩ			
Scope Output Interface	BNC type connector on rear panel for Oscilloscope connection				

OMNIA® II Series

AC POWER SO	OURCE (82X7	only)					
Output	Power:	630 VA and 500	630 VA and 500 W Maximum				
	Voltage:	0 – 150.0 V / 0 –	277.0 V				
	Current:		4.20 A maximum for 0 – 150 V range 2.10 A maximum 0 – 277 V range				
	Distortion:		Hz and output voltage within the 80 ~ 140 ge or the 160 ~ 277 VAC at High Range				
	Regulation:		sistive load), from no load to full load and n Line (combined regulation)				
	Crest Factor:	> 3					
	Test Timing:	< 350 ms at star	t and between				
	Limit:	Steps when inte	rnal AC source is ON				
Settings	Voltage	Low Range:	0.0 – 150.0 V				
		High Range:	0.0 – 277.0 V				
		Resolution:	0.1 V				
		Accuracy:	± (1.5% of setting + 2 counts)				
	Frequency	Range: Resolution: Accuracy:	45.0 Hz – 99.9 Hz 0.1 Hz ± 0.1% of setting				
		Range: Resolution: Accuracy:	100 Hz = 500 Hz 1 Hz ± 0.1% of setting				
	A-HI-Limit	Range: Resolution: Accuracy:	4.20 A / 2.10 A 0.01 A ± (2% of reading + 2 counts)				
Measurement	Voltage	Range: Resolution: Accuracy:	0.0 – 277.0 V 0.1 V ± (1.5% of reading + 2 counts)				
	Current	Range: Resolution: Accuracy:	0.00 – 16.00 A 0.01 A ± (2% of reading + 2 counts)				
	Power	Range: Resolution: Accuracy:	0-4500 1 ± (5% of reading + 3 counts) for PF > 0.100				
	Power Factor	Range: Resolution: Accuracy:	0.000 – 1.000 0.001 ± (8% of reading + 5 counts)				
	Frequency:	Range: Resolution: Accuracy:	45 – 500 Hz 0.1 Hz ± 0.1 Hz				

GENERAL SPECI	FICATIONS			
PLC Remote Control	Input: Test, Reset, Interlock, Recall File 1 through 3 Output: Pass, Fail, Test-in-Process			
Safety	Built-in SmartGFI circuit			
Memory	10,000 Steps			
Interface	Standard: USB/RS-232 Optional: Ethernet or GPIB			
Security	Advanced security system with access levels and username/password requirements			
Dimensions (W x H x D)	16.93" x 5.24" x 19.69" (430 x 133 x 500 mm)			
Weight	8204/8254: 92 lbs (42 kg) 8206/8207: 103 lbs (47 kg) 8256/8257: 103 lbs (47 kg)			

For reading specifications, please refer to the user manual.

Why We Use Counts
Associated Research publishes some specifications using "counts" which allows us to provide a better indication of the instrument's capabilities across measurement ranges. A count refers to the lowest resolution of the display for a given measurement range. For example, if the resolution for voltage is 1V then 2 counts = 2 V.

The default of the Adapter Box accesscoy come in L-N polarity. N-L polarity is available

Specifications subject to change without notice.



Our HYAMP® Series provides manufacturers with data-driven results and greater test flexibility required in today's complex test environment. Quickly collect test data and test settings from the convenient front panel USB port onto a standard USB flash drive. Use the front panel barcode connection to associate products with preprogrammed test files. Test with greater flexibility by performing either AC Ground Bond or DC Ground Bond at a maximum of 40 A of current. The HYAMP® features a drastically reduced weight and footprint making it the ideal lightweight Ground Bond solution for laboratory and production line testing applications. Easily interconnect with the Hypot® Series to form a complete safety compliance system.



Find the Model that Fits Your Testing Needs



3240 AC/DC

SAFETY & PRODUCTIVITY FEATURES







PLC Remote Basic PLC relay control

Interlock
Easily disable
HV output

Data Transfer Easily import/ export test files and data via USB



Barcode Capability Direct barcode



Multiple Languages Multi-Language user interface



Ground Bond Voltage Drop Monitor voltage drop vs resistance



FailCHEKTM Confirms failure detection



Prompt & Hold Provides alerts & instructions between tests



Advanced
User Security
Customize ID
& password
protection







4-Wire Measurement More accurate milliohm measurement



Interconnection Interconnect with Hypot® to form a complete test system



On Board Data Storage Save up to 1,500 Test Results on-



WithStand® Automation Software

INPUT SPECIFICATION	ONS		
Voltage	100 – 120 VAC / 200 – 240 VAC ± 10% Auto Range		
Frequency	50/60Hz ± 5%		
Fuse	10 A, Slow B	low 250 VAC	
GROUND BOND TE	ST MODE		
Output Voltage (Open Circuit Voltage)	Range: Resolution: Accuracy:	3.00 – 8.00 VAC/DC 0.01 VAC/DC ± (3% of setting + 3 counts)	
Output Frequency	50 or 60 Hz,	User Selectable/DC	
Output Current	Range: Resolution: Accuracy:	0 – 150 mΩ for 30.01 – 40.00 A 0 – 200 mΩ for 10.01 – 30.00 A 0 – 600 mΩ for 1.00 – 10.00 A 0.1 A \pm (3% of setting + 3 counts)	
Maximum Loading	Range: Resolution: Accuracy:	1.00 - 10.00 A, $0 - 600$ mΩ 10.01 - 30.00 A, $0 - 200$ mΩ 30.01 - 40.00 A, $0 - 150$ mΩ 1 mΩ \pm (2% of setting + 2 counts)	
HI and LO-Limit Resistance	Range: Resolution: Accuracy:	0 – 150 mΩ for 30.01 – 40.00 A 0 – 200 mΩ for 10.01 – 30.00 A 0 – 600 mΩ for 1.00 – 10.00 A 1 mΩ \pm (2% of setting + 2 counts)	
HI and LO-Limit Voltage	Range: Resolution: Accuracy:	0.00 – 6.00 V 0.01 ± (2% of settings + 2 counts)	
Dwell Time Setting	Range:	0, 0.5 – 999.9 sec (0=Continuous)	
Ω Offset Capability	Range: Resolution: Accuracy:	0 - 100 mΩ 1 mΩ \pm (2% of setting + 2 counts)	
V Offset Capability	Range: Resolution: Accuracy:	0.00 – 4.00 V 0.01 V ± (2% of setting + 2 counts)	
Current Display	Range: Resolution: Accuracy:	0.00 – 40.00 AAC/DC 0.01 AC/DC ± (3% of reading + 1 count)	
Voltage Display	Range: Resolution: Accuracy:	0.00 - 8.00 VAC/DC 0.01 AC/DC ± (2% of reading + 2 counts)	
Ohmmeter Display	Range: Resolution: Accuracy:	$0-600$ mΩ for $1.00-5.99$ A 1 mΩ \pm (3% of reading $+3$ counts)	
	Range: Resolution: Accuracy:	0 – 600 mΩ for 6 – 40 A 1 mΩ ± (2% of reading + 2 counts)	

GENERAL SPECIFICATIO	GENERAL SPECIFICATIONS		
Remote Control and Signal I/O	The following input and output signals are provided through two 9 pin D type connectors: Inputs: Test, Reset, Hardware Interlock, File Recall Outputs: Pass, Fail, Test-in-Process, Reset-Out, Start-Out Hardware Interlock (safety)		
Memories	50 steps 1500 test results		
Interface	USB standard		
Language	English, Traditional Chinese, Simplified Chinese, Turkish, Portuguese, Spanish, German, French		
Security	Multiple user setups with ID and password		
Dimensions (W x H x D)	8.5" x 3.5" x 11.9" (215 x 88.1 x 300 mm)		
Weight	11 lbs (5 kg)		

For reading specifications, please refer to the user manual.

Why We Use Counts

Associated Research publishes some specifications using "counts" which allows us to provide a better indication of the instrument's capabilities across measurement ranges. A count refers to the lowest resolution of the display for a given measurement range. For example, if the resolution for voltage is 1V then 2 counts = 2 V.

 ${\bf Specifications\ subject\ to\ change\ without\ notice.}$



Our HypotMAX® Series is a complete line of automated Hipot instruments designed to meet the demanding requirements of high voltage applications. We've included our patented SmartGFI® feature for maximum operator safety as well as a variety of advanced features to increase productivity on the production line and in the lab. Set up and run tests with confidence from our intuitive user interface or automate with a PC.



AVAILABLE INTERFACES







SAFETY & PRODUCTIVITY **FEATURES**







PLC Remote Basic PLC relay control

Automatic operator shock protection

Remote Safety Interlock Easily disable HV output



Arc Detection

High frequency

detection





Ramp-HI® Reduce ramp

time during DC Hipot

Confirms proper DUT connection





Accredited Accredited calibration options available

WithStand® Automation Software

Find the Model that Fits Your Testing Needs



7715	•	
7720		•

INPUT SPECIFICATIONS		
Voltage	115/230 VAC ± 10%, Single Phase, User Selection	
Frequency	50/60 Hz ± 5%	
Fuse	6.3 A, 250 V Slow Blow	

Frequency	50/60 Hz ± 5%		
Fuse	6.3 A, 250 V Slow Blow		
DIELECTRIC WITI	HSTAND TE	ST MODE	
Output Rating	7705: 7710: 7715: 7720:	10 kV @ 20 mA 12 kV @ 10 mA 20 kV @ 10 mA 20 kV @ 5 mA	DC AC
HI-Limit and LO-Limit	7705	Range 1: Resolution: Range 2: Resolution:	0.0 – 9.999 mA 0.001 mA 10.00 – 20.00 mA 0.01 mA
	7710	Range 1: Resolution: Range 2: Resolution:	0.00 – 999.9 μA 0.1 uA 1,000 – 9,999 μA 1 μA
	7715	Range: Resolution:	0.00 – 9.999 mA 0.001 mA
	7720	Range 1: Resolution: Range 2: Resolution:	0.0 – 999.9 μA 0.1 μA 1,000 – 5,000 μA 1 μA/step
	77XX	Accuracy:	± (2% of setting + 2 counts)
DC Ramp HI	7710	13 mA peak m	aximum, 10 mADC, ON/OFF selectable
	7720	6.75 mA peak	maximum, 5 mADC, ON/OFF selectable
DC Charge LO	7710/7720	Range:	$0.0-350~\mu\text{ADC}$ or auto set
Arc Detection	7705		voltage < 7.00 kV voltage ≥ 7.00 kV
	7710/7720	1 – 9	
	7715		voltage < 15.00 kV voltage ≥ 15.00 kV
Voltage Display	7705	Range: Accuracy:	0.00 – 10.00 kV Full scale ± (1.5% of reading + 20 V)
	7710	Range: Accuracy:	0.00 – 12.00 kV Full scale ± (1.5% of reading + 20 V)
	7715/7720	Range: Accuracy:	0.00 – 20.00 kV Full scale ± (1.5% of reading + 20 V)
Current Display	7705	Auto Range Range 1: Range 2:	0.000 – 3.500 mA 3.00 – 20.00 mA
	7710	Auto Range Range 1: Range 2: Range 3:	0.0 – 350.0 μA 300 – 3500 μA 3,000 – 9,999 μA
	7715	Auto Range Range 1: Range 2:	0.000 – 3.500 mA 3.00 – 10.00 mA
	7720	Auto Range Range 1: Range 2:	0.0 – 350.0 μA 300 – 5,000 μA
DC Output Ripple	7710	< 5% Ripple at	: 12 kV @ 9,999 μA, Resistive Load
	7720	< 5% Ripple at	20 kV @ 4,999 μA, Resistive Load
AC Output Waveform	Sine Wave, 0	Crest Factor = 1.	3 – 1.5
Output Frequency	Range:	50/60 Hz, User ± (1% of outpu No load to full	t + 5 V) from Regulation
Output Regu- lation	± (1% of out	put + 10 V) from	no load to full load
Discharge Timer	7710	No load < 400	ms
	7720	No load < 500	ms
Dwell Timer	Range: 0, 0.3 – 999.9 sec (0=Continuous) AC Range: 0, 0.3 – 999.9 sec or min (0=Continuous)		0, 0.3 – 999.9 sec (0=Continuous) 0, 0.3 – 999.9 sec or min (0=Continuous) 0, 0.4 – 999.9 sec or min (0=Continuous)
Ramp Timer	7705/7715	Range:	0.3 – 999.9 sec
	7710/7720	Range:	0.4 – 999.9 sec
Ground Conti- nuity	Max. Ground	d Resistance 1 Ω	2 ± 0.1 Ω, fixed

DIELECTRIC WITHSTAND TEST MODE		
Ground Fault Interrupt	HV Shut Down Speed < 1 ms GFI Trip Current 1 mA max	
GENERAL SPECIFICATIONS		
Memory	50 memories w/ 8 steps per memory	
Mechanical	Tilt-up front feet	
Interface	Standard: USB, RS-232 Optional: GPIB	
Dimensions (W x H x D)	16.93" x 5.24" x 15.75" (430 x 133 x 400 mm)	
Weight	7705: 63.3 lb (28.7kg) 7710: 63.1 lb (28.6kg) 7715: 59.4 lb (26.9kg) 7720: 61.6 lb (27.9 kg)	

For reading specifications, please refer to the user manual.

Why We Use Counts
Associated Research publishes some specifications using "counts" which allows us to provide a better indication of the instrument's capabilities across measurement ranges. A count refers to the lowest resolution of the display for a given measurement range. For example, if the resolution for voltage is 1V then 2 counts = 2 V.


Specifications subject to change without notice.



Our patented SC6540 multiplexer pioneered the largest productivity improvement in the electrical safety compliance industry in years. With up to 16 independent high voltage or high current channels in a convenient 2U design, the SC6540 can be customized in 10 different configurations for multi-point Hipot, Ground Bond, Insulation Resistance, and Leakage Current testing. Configure the SC6540 according to your needs, and interface with your OMNIA® II, HypotULTRA® or LINECHEK® II instrument to improve production line throughput or expand lab testing capability. Operate from the front panel of your AR instrument or utilize a variety of automation interfaces for direct PC control.



Find the Model that Fits Your Testing Needs

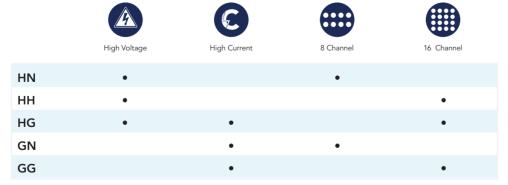

Available in both main and secondary configurations

AVAILABLE INTERFACES









PRODUCTIVITY ENHANCING FEATURES





Interconnection
Interconnect
with the
HypotULTRA®,
OMNIA® II or
LINECHEK® II to
form a complete
test system

Automation Software

FOR USE WITH THE FOLLOWING TESTS







AC Hipot

DC Hipot

Ground Bond







Insulation Resistance

Current

MODULAR MULT	IPLEXER SP	PECIFICATIONS	
Input (Main only)	115 VAC (± 10%), 50/60 Hz, single phase 230 VAC (± 10%), 50/60 Hz, single phase User selectable		
Fuse (Main only)	250 V/2 A/fa	st-blow	
PC Control (Main only)		Standard: USB, RS-232 Optional: Ethernet, GPIB	
Multiplexer Control	Main: One Multiplexer bus output controls, up to 4 additional secondaries Secondary: One output and one input		
Maximum HV Rating	5 kV AC and DC		
Maximum HC Rating	40 A		
Number of Possible Channels	8 or 16		
HV Output	100' reel HV cable rated for up to 30 kV Terminations with 8 HV connectors		
GND Output	20 terminals provided, to accept 10/12 AWG Terminations hook-up wire (user supplied wire)		
Temperature	32° – 104° F (0° – 40° C)		
Humidity	0 – 80%		
Altitude	6,560 ft. (2,000 m)		
Mechanical	2U with tilt-up front feet		
Dimensions (W x H x D)	17" x 4.07" x 12.96" (432 x 103 x 329 mm)		
Weight	Main: Secondary:	20.05 lbs. max. (9.09 kg) (with 2 high voltage modules) 15.45 lbs. max. (7.01 kg) (with 2 high voltage modules)	

CONFIGURATIONS

The modular design can be customize to fit your application. In addition to main or secondary control, the SC6540 can be set up in the following configurations: 8 or 16 high voltage channels, 8 or 16 high current channels, and 8 high voltage channels and/or 8 high current channels. Refer to the images for details.

The different configurations (shown below) are indicated by the following alpha designators

M – Main Multiplexer H – 8 High Voltage Channels HH – 16 High Voltage Channels

G – 8 Ground Bond Channels GG – 16 Ground Bond Channels

N – Empty Module

S – Secondary



MODEL SC6540 HNM*

8 Channel High Voltage Multiplexer



MODEL SC6540 HHM*

16 Channel High Voltage Multiplexer



MODEL SC6540 HGM*

8 Channel High Voltage Multiplexer 8 Channel High Current Multiplexer



MODEL SC6540 GNM*

8 Channel High Current Multiplexer




MODEL SC6540 GGM*

16 Channel High Current Multiplexer

 ${\rm *Also~available~in~secondary~configuration}$



Our LINECHEK® II model 620L provides 7 measuring devices (MD's) compliant with international certification bodies as well as a convenient switching network to simulate all 8 required fault conditions, everything you need for full Leakage Current compliance. Utilize the intuitive user interface or control via a PC for more advanced automated applications that require data storage and analysis. The 620L handles up to 40 A of continuous current and can be interfaced to an SC6540 modular multiplexer for multi-point testing. Interconnect the 620L to an OMNIA® II instrument to form a complete electrical safety compliance testing system.

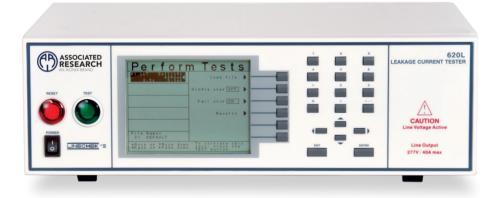

AVAILABLE INTERFACES









Ethernet (Optional)

SAFETY & PRODUCTIVITY FEATURES







Prompt & Hold Provides alerts & instructions between tests

Remote Safety Interlock Easily disable HV output

Active Link® Continuous power during test steps







PLC Remote Basic PLC relay control

Modular Multiplexer Compatible with SC6540 multiplexers

Interconnection
Interconnect
with OMNIA®
II or HypotULTRA® to form a
complete test
system





Cal-Alert® Tracks and alerts for calibration

WithStand® Automation Software

Find the Model that Fits Your Testing Needs



eakage Current



unctiona



620L

•

•

.

	ATIONS		
Voltage	115/230 VAC ± 10%, User Selection		
Frequency	50/60 Hz ± 5%		
Fuse	2 A Slow Blo	w 250 VAC	
LINE CONDITION	NS		
Reverse Power Switch	Switch for po	ower polarity reversal	
Neutral Switch	Neutral switch	ch on/off selection for single fault	
Ground Switch	Ground swite	ch on/off selection for class I single fault	
PROBE SETTING	S		
Surface to Surface	(PH – PL)		
Surface to Line	(PH – L)		
Ground to Line	(G – L)		
LEAKAGE LIMIT	SETTINGS		
Touch Current	Range:	0.0 μA – 999.9 μA / 1,000 μA – 9,999 μA / 10.00 mA – 20.00	
High/Low Limit (rms)	Resolution:	mA 0.1 μA / 1 μA / 0.01 mA	
Touch Current	Range:	0.0 μA -999.9 μA / 1,000 uA – 9,999 μA / 10.00 mA – 30.00	
High/Low Limit (Peak)	Resolution:	mA 0.1 μA / 1 μA / 0.01 mA	
DISPLAY			
Touch Current Display (rms)	Range: Resolution: Accuracy:	0.0 μ A – 550 μ A, frequency DC, 15 Hz – 1 MHz 0.1 μ A DC: 15 Hz \leq f \leq 100 kHz: \pm (2% of reading + 3 counts) 100 kHz \leq f \leq 1 MHz: \pm 5% of reading (10.0 μ A – 999.9 μ A	
	Range: Resolution: Accuracy:	400 μA – 8,500 μA, frequency DC, 15 Hz – 1 MHz 1 μA DC: 15 Hz \leq f \leq 100 kHz: \pm (2% of reading + 3 counts) 100 kHz \leq f \leq 1 MHz: \pm 5% of reading, (10.0 μA – 8,500 μA)	
	Range: Resolution: Accuracy:	8.00 mA $-$ 20.00 mA, frequency DC, 15 Hz $-$ 100 KHz 0.01 mA DC: 15 Hz \le f \le 100 MHz: \pm 5% of reading (0.01 mA $-$ 20.00 mA)	
Touch Current Display (peak)	Range: Resolution: Accuracy:	0.0 μ A – 550 μ A, frequency DC – 1 MHz 0.1 μ A ± (2% of reading + 2 μ A) 15 Hz \leq f \leq 1 MHz, ± 10% of reading + 2 μ A	
	Range: Resolution: Accuracy:	400 μA – 8,500 μA, frequency DC – 1 MHz 1 μA ± (2% of reading + 2 μA) 15 Hz \leq f \leq 1 MHz, \pm 10% of reading + 2 μA	
	Range: Resolution: Accuracy:	8.00 mA − 30.00 mA, frequency DC − 100 kHz 0.01 mA ± (2% of reading + 3 counts) 15 Hz ≤ f ≤ 100 kHz, ± 10% of reading + 2 counts	
MEASURING DE	VICE MODU	LE	
MD1	UL544NP, UL	.484 , UL923, UL471, UL867, UL697	
MD2	UL544P		
MD3	IEC 60601-1		
MD4	UL1563		
MD5	IEC60990 Fig4 U2, IEC62368-1, IEC60335-1, IEC60598-1, IEC60065, IEC61010		
MD6	IEC60990 Fig5 U3, IEC60598-1		
IIIDO		,	

Basic measuring element 1 kohm

External MD

MD Voltage Limit

DUT POWER			
AC Voltage	0.0 – 277.0 V		
AC Current	40 A max con	tinuous	
AC Voltage High/Low Limit	Range: Resolution:	0.0 – 277.0 V 0.1 V/step	
AC Voltage Display	Range: Resolution: Accuracy:	0.0 – 277.0 V 0.1 V/step ± (1.5% of reading + 2 counts), 30.0 – 277.0 V	
Delay Time Setting	Range: Resolution:	0.5 – 999.9 sec 0.1 sec	
Dwell Time Setting	Range: Resolution: Accuracy:	0, 0.5 – 999.9 sec (0=Continuous) 0.1 sec ± (0.1% of reading + 0.05 seconds)	
Failure Protection	On Start-Up – Neutral Voltage Check (Neutral – V) Over current and ground current check (Line – OC)		
GENERAL SPECI	FICATIONS		
Memory	50 Memories, 30 steps per each memory File locations can link 900 steps max		
Mechanical	Bench or rackmount with tilt-up feet		
Interface	Standard: USB, RS-232 Optional: Ethernet, GPIB		
Dimensions (W x H x D)	16.93" x 5.24" x 11.81" (430 x 133 x 300 mm)		
Weight	26.45 lbs (12 kg)		

For reading specifications, please refer to the user manual.

Why We Use Counts

Associated Research publishes some specifications using "counts" which allows us to provide a better indication of the instrument's capabilities across measurement ranges. A count refers to the lowest resolution of the display for a given measurement range. For example, if the resolution for voltage is 1V then 2 counts = 2 V.

The default of the Adapter Box accesscoy come in L-N polarity. N-L polarity is available upon request.

Specifications subject to change without notice.

MedTEST

A Complete Electrical Safety Testing System that Satisfies the Most Demanding **Medical Compliance Requirements**



Our MedTEST system can be designed to provide a complete test solution for medical device manufacturers in need conforming to IEC 60601-1 3rd Edition Standard. Customize your MedTEST system to satisfy your individual testing requirements including Hipot, Ground Bond, Insulation Resistance, Functional Run and leakage current testing for all B, BF and CF type applied parts including Mains on Applied Parts (MOAP) tests. Up to 40 A of continuous DUT current combined with our Active Link® technology reduces overall test time and integration with our modular multiplexer SC6540 allows for multi-point sequential testing without the need to change test leads. Get the most from your test system by utilizing our WithStand® software for maximum productivity-enhancing benefits.



Rack cabinet shown in image is for illustration only. Ikonix does not sell or distribute the rack cabinet.

SAFETY & PRODUCTIVITY FEATURES Hold Automatic Easily disable HV output Provides alerts operator shock protection & instructions between tests





AVAILABLE INTERFACES

Ethernet

RS-232



GPIB

Continuous power during test steps

Mv Menu Customize your own shortcut menu



Languages

Multi-

Language user interface

DualCHEK® Simultaneous Hipot and Ground Bond



Internal Multiplexer Available with optional HV multiplexer



Multiplexer Compatible with SC6540 multiplexers



FailCHEK™

Confirms

failure

detection



Cal-Alert® Ramp-HI® Tracks and Reduce ramp alerts for time during DC calibration Hipot





available





Confirms

Accredited Cal proper DUT connection



Automation Accredited Software calibration











Continuity



Resistance



Current



Run



Recommended













POPULAR MEDTEST CONFIGURATIONS



OMNIA® II 8207 AND SC6540

- All-in-one testing system (Hipot, Ground Bond, Insulation Resistance, and Leakage Current)
- Built in 500 VA AC power source
- Efficient use of rack space
- SC6540 provides automated multi-point testing Most common applications incorporate 8 or 16 port multiplexers



OMNIA® II 8206, SC6540 AND POWERED BY AN OCCUPANT AC POWER SOURCE

- All-in-one testing system (Hipot, Ground Bond, Insulation Resistance, and Leakage Current)
- Compatible EEC power source provides power to DUT*
- SC6540 provides automated multi-point testing.
 Most common applications incorporate 8 or 16 port multiplexers
 *Choose from EEC 8500 Series.



OMNIA® II 8204, 620L, SC6540 AND POWERED BY AN OCCUPANIED AC POWER SOURCE

- All-in-one testing system (Hipot, Ground Bond, Insulation Resistance, and Leakage Current)
- Compatible EEC power source provides power to DUT*
- SC6540 provides automated multi-point testing Most common applications incorporate 8 or 16 port multiplexers
- Up to 40 A continuous current capability for applications that draw greater than 16 A of current

*Choose from EEC 8500 Series.

MedTEST

LINE CONDITION	NS		
Reverse Power Switch	Switch for power polarity reversal		
Neutral Switch	Neutral switch on/off selection for single fault		
Ground Switch	Ground switch on/off selection for class I single fault		
PROBE SETTING	S		
Surface to Surface	(PH – PL)		
Surface to Line	(PH – L)		
Ground to Line	(G – L)		
LEAKAGE LIMIT	SETTINGS		
Touch Current High/Low Limit (rms)	Range:	0.0 μA – 999.9 μA / 1,000 μA – 9,999 μA / 10.00 mA – 20.00 mA 0.1 μA / 1 μA / 0.01 mA	
Touch Current High/Low Limit (Peak)	Range:	0.0 μA -999.9 μA / 1,000 uA – 9,999 μA / 10.00 mA – 30.00 mA 0.1 μA / 1 μA / 0.01 mA	
MEASURING DEVICE MODULE			
MD1	UL544NP, UL484 , UL923, UL471, UL867, UL697		
MD2	UL544P		
MD3	IEC 60601-1		
MD4	UL1563		
MD5	IEC60990 Fig4 U2, IEC62368, IEC60335-1, IEC60598-1, IEC60065, IEC61010		
MD6	IEC60990 Fig5 U3, IEC60598-1		
MD7	IEC62368, IEC61010-1 FigA.2 (2 kohm) for Run function		
External MD	Basic measuring element 1 kohm		
MD Voltage Limit	70 VDC		
DUT POWER			
AC Voltage	0.0 – 277.0 V		
AC Current	40 A max continuous		
AC Voltage High/Low Limit	Range: Resolution:	0.0 – 277.0 V 0.1 V/step	
AC Voltage Display	Range: Resolution: Accuracy:	0.0 – 277.0 V 0.1 V/step ± (1.5% of reading + 2 counts), 30.0 – 277.0 V	
Delay Time Setting	Range: Resolution:	0.5 – 999.9 sec 0.1 sec	
Dwell Time Setting	Range: 0, 0.5 – 999.9 sec (0=Continuous) Resolution: 0.1 sec Accuracy: ± (0.1% of reading + 0.05 seconds)		
Failure Protection	On Start-Up – Neutral Voltage Check (Neutral – V) Over current and ground current check (Line – OC)		

DIELECTRIC WITI	HSTAND TES	T MODE	
Output Rating*	5 kV @ 50 mAAC 6 kV @ 20 mADC		
Voltage Setting	Range: Resolution:	0 – 5,000 VAC, 0 – 6,000 VDC 1 V	
	Accuracy:	± (1.5% of settin	g + 5 V)
HI and LO-Limit	AC Total	Range: Resolution: Accuracy:	0.000-9.999 mA 0.001 mA ± (2% of setting + 2 counts)
		Range: Resolution: Accuracy:	10.00 – 50.00 mA 0.01 mA ± (2% of Setting + 2 counts)
	AC Real	Range: Resolution: Accuracy:	0.000 - 9.999 mA 0.001 mA $\pm (3\% \text{ of setting} + 50 \mu\text{A})$
		Range: Resolution: Accuracy:	10.00 - 50.00 mA 0.01 mA $\pm (3\% \text{ of setting} + 50 \mu\text{A})$
	DC	Range: Resolution: Accuracy:	$0.00 - 999.9 \mu\text{A}$ $0.1 \mu\text{A}$ $\pm (2\% \text{of setting} + 2 \text{counts})$
		Range: Resolution: Accuracy:	1,000 $-$ 20,000 μ A 1 μ A \pm (2% of setting + 2 counts)
Ramp HI	> 20 mA peak maximum, ON/OFF selectable		
Charge LO	Range: 0.000 – 350.0 μA or Auto Set		
DC Output Ripple	\leq 4% Ripple rms at 5 kVDC @ 20 mA, Resistive Load		
Discharge Timer	< 50 msec for no load, < 100 msec for capacitor load (All capacitance values in MAX load spec below)		
Maximum Capacitive Load	1 μF < 1 kV 0.08 μF < 4 kV 0.75 μF < 2 kV 0.04 μF < 6 kV 0.50 μF < 3 kV		
Output Frequency	50/60 Hz ± 0.1	% , User Selection	n, 400/800 Hz Option
AC Output Waveform	Sine Wave, Crest Factor = 1.3 – 1.5		
Output Regu- lation	\pm (1% of output + 5 V) from no load to full load and over input voltage range		oad to full load and over input
Dwell Timer	AC 0, 0.4 – 999.9 sec (0=Continuous) DC 0, 0.3 – 999.9 sec (0=Continuous)		
Ramp Timer	Ramp-Up AC: 0.1 – 999.9 Ramp-Down AC: 0.0-999.9 Ramp-Up DC: 0.4 – 999.9 Ramp-Down DC: 0.0, 1.0-999.9		
Ground Conti- nuity	Current: DC 0.1 A \pm 0.01 A, fixed Max. Ground Resistance: 1 Ω \pm 0.1 Ω , fixed		
Ground Fault Interrupt	GFI Trip Current: 5.0 mA max HV Shut Down Speed: < 1 ms		

^{*}Output voltage limited to 3.5 kV with 620L option 03 $\,$

CONTINUITY TE	ST MODE		
Output Current	DC 0.1 A ± 0.00001 A		
Resistance Display	Range:	0.00 – 10,000.00 Ω	
HI and LO-Limit	0.00 – 10,000 Ω	2	
Dwell Timer	Range:	0.0, 0.3 – 999.9 sec (0=Continuous)	
Milliohm Offset	Range:	0.00 – 10.00 Ω	
GROUND BOND	TEST MODE		
Output Voltage	Range:	3.00 – 8.00 VAC	
Output Frequency	50/60 Hz ± 0.1%	6, User Selection	
Output Current	Range: Resolution: Accuracy:	1.00 – 40.00 A 0.01 A ± (2 % of setting + 2 counts)	
Output Regu- lation	\pm (1% of output + 0.02 A) Within maximum load limits, and over input voltage range		
Maximum Loading	1.00 - 10.00 A, $0 - 600$ mΩ $10.01 - 30.00$ A, $0 - 200$ mΩ $10.01 - 40.00$ A, $0 - 150$ mΩ		
HI and LO-Limit	Range:	0 – 150 for 30.01 – 40.00 A	
	Range:	0 – 200 for 10.01 – 30.00 A	
	Range:	0 – 600 for 6.00 – 10.00 A	
	Range:	0 – 600 for 5.99 – 1.00 A	
	Resolution:	1 mΩ	
	Accuracy:	6.00 – 40.00 A, ± (2% of setting + 2 Counts) 1.00 – 5.99 A, ± (3% of setting + 3 Counts)	
Milliohm Offset	Range:	0 – 200 mΩ	
INSULATION RES	SISTANCE TES	T MODE	
Output Voltage	Range:	30 – 1,000 VDC	
Charging Current	Maximum > 20	mA peak	
HI and LO-Limit	Range: Resolution:	0.05-99.99 MΩ 0.01 MΩ	
	Range: Resolution:	100.0 – 999.9 MΩ 0.1 MΩ	

Range: $1000 - 50,000 \text{ M}\Omega$ Resolution: $1 \text{ M}\Omega$

 $0.000-3.500~\mu\text{A}$ or Auto Set Ramp Up: 0.1 – 999.9 secs Ramp Down: 0.0, 1.0 – 999.9 secs

0, 0.5 – 999.9 (0=Continuous)

GFI Trip Current: 5.0 mA max

HV Shut down Speed: < 1 ms

0.5 - 999.9 secs

Charge-LO

Ramp Timer

Dwell Timer Delay Timer

Ground Fault

Interrupt

GENERAL SPECIFICATIONS				
Interface	Standard: USB, RS-232 Optional: Ethernet, GPIB			
Safety	Built-in SmartGFI® circuit			
Memory	620L: 50 memories, 30 steps per memory OMNIA® II: 10,000 steps			
AC POWER SOURCE				
AC Power Source	Up-to 6 kVA compatible power sources available			
Configuration	AC Power Source configuration depends on application. MedTEST hardware is configured for testing products with one side of the supply mains at earth potential (Fig 10 UL60601-1). MedTEST hardware is configured for unbalanced 0-277 V DUT input power. Custom Configurations available. Contact us for details.			

For reading specifications, please refer to the user manual.

Why We Use Counts

Associated Research publishes some specifications using "counts" which allows us to provide a better indication of the instrument's capabilities across measurement ranges. A count refers to the lowest resolution of the display for a given measurement range. For example, if the resolution for voltage is 1V then 2 counts = 2 V.

Specifications subject to change without notice.




Interconnect our Hypot® Series Hipot Instrument with our HYAMP® Series Ground Bond instrument to form a complete safety compliance system. Easily operate both instruments from a single point of control on the production line or in a rack. All test systems are safety agency listed, include interconnect cables, and detailed directions on effortlessly interconnecting your system.

	Hypot® 3805	Hypot® 3855	Hypot® 3870			
	AC Hipot	AC Insulation Hipot Resistance	AC DC Hipot Hipot	AC DC Insulation Hipot Hipot Resistance		
HYAMP® 3240						
Ground Bond	System 32-05	System 32-55	System 32-65	System 32-70		

SETTING UP A SAFE WORKSTATION

Setting up a safe and secure workstation is one of the best ways to protect your test operators. You can setup test stations with or without direct protection depending on your requirements.

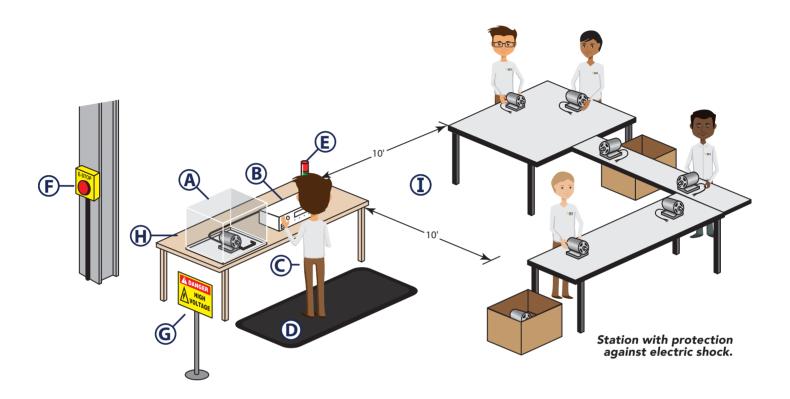

	Description
А	DUT Safety Enclosure - This is wired to the Hipot tester's Remote Safety Interlock. This protects you from touching the DUT while a test is in progress. When you open the enclosure door, it will immediately disable the instrument's high voltage output.
В	Hipot Tester – Performs test on the DUT
С	Test Operator
D	High Voltage Insulation Mat – This isolates you from ground which provides an additional means of protection when operating high voltage equipment.
Е	Signal Tower Light – Gives an indication as to the status of the testing area. A green light indicates the Hipot instrument is not outputting high voltage and the test area is safe. A red light indicates that the Hipot instrument is active and to stay clear of the test area.
F	Emergency Stop Button – An E-stop button is located on the perimeter of the test area. In the event of an emergency, someone outside the test area can hit the E-Stop button to immediately cut off power to the entire test station.
G	Warning Signs – Mark the testing area with clearly posted signs that read: DANGER-HIGH VOLTAGE TEST AREA. AUTHORIZED PERSONNEL ONLY.
Н	Non-Conductive Work Bench – Only use a work bench made of non-conductive material such as plastic or wood. This ensures no stray leakage current could flow through you during a test.
I	NEC (National Electric Code) and NFPA (National Fire Protection Agency) stipulate that any unqualified workers shall not come within 10 feet of an EXPOSED energized circuit.

ESSENTIAL WORKSTATION PPE & ACCESSORIES

Class 3 Insulation Mat 40396

Thickness: 3/8" (9.53 mm)

Dimensions: 3' x 3' (91.44 x 91.44 cm)



High Voltage Warning Sign 39538



DUT Enclosure Wood Frame with Foam Interior 39067

Protect your operator from electric shock by enclosing your DUT. Our enclosures automatically disable the instrument's output when the enclosure door is opened. Our DUT Enclosures are designed to protect the operator from electric shock during testing. Interface an enclosure with our Remote Safety Interlock feature to automatically disable the instrument's output when the enclosure door is opened.

Outside dimensions (W x D x H): 24" x 19" x 11.5" (610 x 483 x 293 mm) Inside dimensions (W x D x H): 20" x 16" x 10" (508 x 407 x 254 mm) 3/4" Walls, 3/4" Flame Retardant Foam, 1/4" Plexiglass cover



Dual Palm Remote Switch

DPR-01

Prevent your operator from touching a DUT as their hands must stay on the test switches to continue to run a test.



Remote Test Box w/LED Indicators

RTB-02

Helps maintain a safe distance between the operator and test instrument when starting and restarting a test. Compatible with all models except SC6540.



E-Stop ESTOP

Immediately stop the flow of electric current to your instrument when the E-Stop is triggered. The E-Stop provides the safest and fastest way for a rescuer to save an operator from injury.



Test Verification Box TVB-2

The TVB-2 is a go/no-go daily test verification box designed to ensure that the failure detectors of an Associated Research electrical safety testing instrument are functioning properly. We designed the TVB-2 to verify Hipot, Insulation Resistance, Ground Bond, and Ground Continuity test functionality. If you perform daily verifications on your testing equipment, then the TVB-2 is an ideal solution. An accessory cord is available to customers who prefer to verify their test instrument using an adapter box.



CE

TVB-2 Accessory Cord 39514

Accessory line cord for the TVB-2 allows convenient connection to a standard adapter box.



Leakage Current Verification Box LVB-2

Verify the failure detectors of your Associated Research Leakage Current Test instrument are functioning properly with this go/no-go load box.



Signal Tower Light 24V 40417

Our Signal tower light gives operators a visual indication of the status of the testing area. A green light indicates the Hipot tester is not outputting high voltage and the test area is safe. A red light indicates that the Hipot tester is active and to stay clear of the test area. Compatible with OMNIA® II Series, HypotULTRA® Series, Hypot® Series, HYAMP® Series, HypotMAX® Series, and LINECHECK II (620L).



Magnetic Hipot Return Cable CBLSR-05M



2 Wire 40A Ground Bond Probe 38539

4 Wire 40A Ground Bond Probe 38538



High Voltage Pistol Probe with Switch 38814



High Voltage Probe 38081

Return Probe 38082



COMMON SAFETY STANDARD REFERENCE CHART

Standard/	Testing Type	Dielectric Withstand			Ground Bond/Continuity				
Harmonized Standard		Test Voltage	Max I.	Test Time	Test Current	V Limit	Max. R	Test Time	
IEC/UL 60601-1 3rd Edition	Performance	500 – 4000 VAC or 707 – 5656 VDC	No Breakdown	60 s	10-25 A	≤ 6 V	≤ 0.1 Ω	5 s	
Medical Electrical Equipment	Production*	1000 – 3000 VAC		1 or 60 s	10-25 A	≤ 6 V	≤ 0.1 Ω	5 s	
IEC 61730-2 UL 1703	Performance	1000 VAC + 2 x rated V or 2000 VAC + 4 x rated V	50 uA	60 s	2.5 x Max Over Current Protection	≤ 12 V	≤ 0.1 Ω	120 s	
Photovoltaic Modules & Panels	Production	1000 VAC + 2 x rated V or (1000 VDC + 2 x rated V) X 120%	50 uA	1 or 60 s	Continuity				
IEC 60335-1 Household	Performance	500 – 2400 VAC x rated V + 2400 VAC	No Breakdown	60 s	≥ 10 A	≤ 12 V	0.1 – 0.2 Ω	≤ 120 s	
Electrical Appliances	Production	400 – 2500 VAC	5-30 mA	1 s	≥ 10 A	≤ 12 V	0.1 – 0.2 Ω	No time specified	
UL 60335-1 Household	Performance	500V – 2400 VAC x rated V + 2400 VAC	No Breakdown	60 s	40 A	≤ 6.5 V	≤ 0.5 Ω	120 s	
Electrical Appliances	Production	400 – 2500 VAC	5-30 mA	1 s	40 A	≤ 12 V	0.1 – 0.2 Ω	No time specified	
IEC 60598-1	Performance	500 – 4 x rated V + 2000 VAC	No Breakdown	60 s	≥ 10 A	≤ 12 V	≤ 0.5 Ω	60 s	
Luminaires	Production		Not	t Specified – Resp	onsibility of Manufact	urer			
UL 1598 Luminaires	Performance	1000 VAC – 1000 VAC x 2 x rated V	No Breakdown	60 s	30 A	≤ 4 V	≤ 0.1 Ω	120 s	
	Production	1200 VAC		1 s	Continuity ≤ 0		≤ 0.1 Ω	Continuity	
IEC/UL 61010-1 & CSA 22.2 No.	Performance	840 – 11940 VAC or 1200 – 7500 VDC	No Breakdown	5 – 60 s	25 or 30 A	≤ 10 V or ≤ 12 V	\leq 0.1 Ω or $<$ 4 V 0.133 Ω	60 or 120 s	
61010-1 Laboratory Control Test & Measurement Equipment	Production			5 s max ramp up 2 s dwell	Continuity				
EN 60204-1 Electrical	Performance	2 x rated V or 1000 VAC	No Breakdown	1 s	0.2 – 10 A	≤ 24 V	Refer to Section 18.2.2	No time specified	
Equipment of Machines	Production	Not Specified – Responsibility of Manufacturer							
UL 2202 Electric Vehicle Charging	Performance	500 VAC or 1000 VAC + 2 x rated V	No Breakdown	60 s	≤ 60 A	≤ 12 V	Continuity	120 – 240 s	
System Equipment	Production	1000 – 1700 VAC + 3.4 x rated V			Continuity				
IEC 61851-1 Electric Vehicle Conductive	Performance	1200 VAC + rated V or DC Equivalent	No Breakdown	60 s		Conti	nuity		
Charging System	Production	Not Specified – Responsibility of Manufacturer							
IEC 62368-1 Audi/Video,	Performance	1000 – 3000 VAC or 1414 – 4242 VDC	No Breakdown	60 s	≤ 40 A	≤ 12 V	≤ 0.1 Ω	60 s	
Information & Communication Technology Equipment	Production			1 – 6 s	Continuity				

^{*}As a result of performing risk analysis, many medical device manufacturers are performing leakage tests as part of 100% production line testing.

Standard/	Testing	Suggested Model	Insulation Resistance			Earth Leakage		
Harmonized Standard	Туре	AR Instrument	Min. R	V Limit	Test Time	Max I.	Test Voltage	
IEC/UL 60601-1 3rd Edition	Performance	8206, 8207, 8256, 8257 or MedTEST	N/A			5-10 mA	110% x rated V	
Medical Electrical Equipment	Production*	7804 or 7854	N/A			5-10 mA	110% x rated V	
IEC 61730-2 UL 1703	Performance	3240, 8206, 8207, 8256, 8257 or MedTEST	10 uA – 1 mA 500 VDC or 40-400 MΩ Max rated V		10 uA – 1 mA	Max rated V		
Photovoltaic Modules & Panels	Production	3240, 3870 or 7850		N/A			N/A	
IEC 60335-1 Household	Performance	8256 or 8257		N/A		0.25 – 5.0 uA	1.06 x rated V	
Electrical Appliances	Production	7804		N/A				
UL 60335-1 Household	Performance	8256 or 8257		N/A		0.25 – 5.0 uA	1.06 x rated V	
Electrical Appliances	Production	7804		N/A				
IEC 60598-1 Luminaires	Performance	8206, 8207, 8256 or 8257	1-4 ΜΩ	500 VDC	60 s	0.5 – 10 mA	Rated V	
Luminaires	Production	Hypot® or 7850		acturer	onsibility of Manuf	ot Specified – Respo	No	
UL 1598 Luminaires	Performance	7804 or 7854	≥ 2 MΩ	500 VDC	No time specified		N/A	
	Production	Hypot® or 7850		N/A			N/A	
IEC/UL 61010-1 & CSA 22.2 No.	Performance	8256, 8257 or MedTEST	N/A			0.5 mA	< 300 V	
61010-1 Laboratory Control Test & Measurement Equipment	Production	3865 or 7850	N/A					
EN 60204-1 Electrical Equipment	Performance	7804 or 7854	≥ 1 MΩ	500 V	No time specified		N/A	
of Machines	Production	Hypot® or 7850		Not Specified – Responsibility of Manufacturer				
UL 2202 Electric Vehicle Charging	Performance	8206, 8207, 8256, 8257 or MedTEST	N/A			0.5 – 0.75 mA or 5 mA	Rated V	
System Equipment	Production	Hypot® or 7850		N/A				
IEC 61851-1 Electric Vehicle Conductive	Performance	8206, 8207, 8256, 8257 or MedTEST	≥ 1 MΩ or ≥ 7 MΩ	500 V	60 s	nly		
Charging System	Production	Hypot® or 7850		Not Specified – Responsibility of Manufacturer				
IEC 62368-1 Audi/Video,	Performance	8206, 8207, 8256, 8257 or MedTEST	≥ 2 MΩ	500 V	60 s	0.25 – 3.5 mA	< 300 V	
Information & Communication Technology Equipment	Production	Hypot® or 7850		N/A				



Ikonix Calibration



Ikonix has developed a comprehensive solution that not only provides top-quality, precise instruments but also ensures swift calibration, guaranteeing instrument accuracy and precision throughout its service life. Ikonix's calibration service is available in two types: ISO Calibration and Standard Calibration. We recommend Associated Research, SCI Electric Safety Tester, and EEC AC Power Source be returned annually for calibration and inspection at our A2LA Accredited ISO 17025 Calibration Lab.

Calibration Benefits

Rapid Turnaround: Fast 5-business-day calibration. If the instrument requires repair during the calibration process, the 5-business-day period will restart, covering both repair and calibration.

Cost Saving: Our one-stop service for verification, calibration, and adjustment eliminates the need to send instruments back and forth between the calibration lab and the original manufacturer for recalibration.

Traceability and Accuracy: We provide certification ensuring that calibration, measurements, and adjustments are not only accurate but traceable to a National Institute of Standards and Technology (NIST).

Full-Scope Calibration: Our calibration is conducted based on Associated Research, SCI Electric Safety Tester, and EEC AC Power Source specification scope, ensuring a thorough calibration and adjustment across all measurement ranges, rather than merely calibrating a few basic points.

Extended Warranty: Annual calibration with Ikonix qualifies your Associated Research, EEC, and SCI branded products for an additional year of coverage beyond the original 5-year warranty* through the extended warranty program. This program also extends coverage for 5 years beyond the instrument's discontinuation date.

*APAC-only products come with a 2-year warranty. The extended warranty does not apply to EEC electrical safety testers sold before 2023. For further details, please contact our sales team.

Types of Calibration

ISO Calibration

Accredited calibrations provide measurement data and uncertainty traceable to the NIST. The Ikonix ISO 17025 calibration laboratory is accredited by the A2LA, and its reports are highly recognized internationally, making them vital to multinational companies and export-oriented industries. If an auditor visits your facility, you can present this calibration to them.

Standard Calibration

Standard Calibration is our base calibration type and provides a certificate stating that Associated Research, EEC, and SCI branded products are calibrated using standards traceable to the NIST.



Record, track and store your data with our brand new software as a service.

Compatible with the Associated Research Hypot® Series, Hypot-ULTRA® Series, OMNIA® II Series (including OMNIA models 8206 or 8256 with the eec 8500 Series), HYAMP® Series, HypotMAX® Series, LINECHEK® II, and SC6540. Also compatible with SCI's 290 Series, 260 Series, and 440 Series.



- Unlimited Users
- Remote Instrument Connection
- Barcode Connection
- Multi-language Support

- Intuitive User Interface
- Cloud / Local Storage
- Auto-File Loading



The platform's interface introduces an intuitive user experience making it easy to setup, run tests and view your reports.



Cloud storage ensures that your tests and data will never be lost or altered – all information is stored immediately to the cloud for access at any time.

Try it out for yourself with a free 30-day trial withstand.ikonixusa.com/auth/signup/create



OUR CONSULTING PACKAGES

Digital Packages

A web-based learning program. Choose from 2 packages; our Consulting on Demand or Customized Digital Package.

On-site Training Package

1-4 day on-site, handson training for your production line or R&D lab.

On-site Validation Package

2 or 4 day on-site training to completely satisfy your organization's validation needs.

*APAC Region Availability: Digital Packages and 1-Day On-site Training Program.

Visit **ikonixasia.com/consulting** to learn how we can help your team WE WILL HELP MAKE SURE YOUR SYSTEM IS SAFE AND EFFECTIVE





HEADQUARTERS

28105 N. Keith Drive Lake Forest, IL 60045 USA **Telephone** +1-847-367-4077 Fax +1-847-367-4080 Email info@ikonixusa.com www.ikonixusa.com

Ikonix Taiwan

12F-2., No.237, Sec. 1, Datong Rd., Xizhi Dist., New Taipei City 221, Taiwan Telephone +886-2-21653066 Fax +886-2-21653077 Email contact@ikonixasia.com www.ikonixasia.com

Ikonix Asia

Unit D3-5-2 (2ND Floor) Block D3, Dana 1 Commercial Centre, Jalan PJU 1A/46, 47301 Petaling Jaya, Selangor, Malaysia Telephone +60-3-78429168 Fax +60-3-78426168 Email contact@ikonixasia.com www.ikonixasia.com







We Have Local Sales Offices Throughout the World

To find your nearest representative visit us at ikonixasia.com